



INDIAN INSTITUTE OF SCIENCE EDUCATION AND RESEARCH

An Autonomous Institution, Ministry of Human Resource Development, Govt. of India.

Dr. Homi Bhabha Road,

Pashan Pune – 411008.

Tel : +91-020-25898017

Fax : +91-020-2589 8186

Website : www.iiserpune.ac.in

OPEN TENDER NOTICE NO: 02/2016

Indian Institute of Science Education and Research (IISER), Pune, an autonomous Institute established under Ministry of HRD, Government of India. IISER is devoted to both teaching and research of the highest caliber in a totally integrated way. IISER, Pune would like to procure the following equipment for its day to day research. The Technical Specifications are given in **Chapter 4: Schedule of Requirements/Specifications and Allied Technical details** are appended herewith.

- **Items** : **Airshower & Garment box for Animal Housing**
- **Tender Enquiry No** : **IISER-PUR- 0225-16**
- **Pre-bid Conference Time& Date** : **11.00 AM to 12.00 PM on 30.06.2016**
- **Time and Date of Submission:** **Before 3.00 PM on 20.07.2016**
- **Time and Date of opening Technical Bid:** **At 03.30 PM on 20.07.2016**

Prospective BIDDERS may submit their offers to The Director, Indian Institute of Science Education and Research, Dr. Homi Bhabha Road, Pashan, Pune – 411 008, India

INDEX

SI No	Heading	Page No
1	Invitation for bids	3
2	Instructions to BIDDERS	11
3	Conditions of contract	17
4	Schedule of requirements, specifications and allied technical details	25
5	Price Schedule – (commercial bid)	27
6	Annexure – A - Format/Questionnaire For Compliance Of Terms And Conditions	55
7	Annexure – B - format of compliance statement of specifications	59
8	Annexure – C - BID SECURITY FORM	60
9	Annexure – D - MANUFACTURER'S AUTHORIZATION FORM	61
10	Annexure – E - PREVIOUS SUPPLY ORDERS FORMAT	62
11	Annexure – F - BIDDER INFORMATION FORM	63

CHAPTER-1. INVITATION FOR BIDS

1. Indian Institute of Science Education and Research (IISER), Pune invites sealed tenders for Airshower & Garment box for Animal Housing. The Technical Specifications are given in Chapter 4: Schedule of requirements/Specifications and allied Technical details .

2. The BIDDERS are requested to give detailed tender in their in two Bids i.e

Part - I: Technical Bid.

Part - II: Commercial Bid.

3. **Contact for information:**
Technical & Commercial contact: Assistant Registrar (Stores & Purchase)
Indian Institute of Science Education and Research (IISER), Pune
Dr. Homi Bhabha Road,
Pashan
Pune – 411 008, India
Tel: +91-020-25908017
Website: www.iiserpune.ac.in
4. **A Pre-bid conference will be held at IISER Pune, Purchase Section, Dr. Homi Bhabha Road, Pashan , Pune – 411008 on 30.06.2016 from 11.00AM to 12.00 PM (IST). All prospective bidders are requested to kindly submit their queries to the address indicated above or email at purchase@iiserpune.ac.in so as to reach latest by 29.06.2016. During Pre-bid meeting the answers / clarifications to the queries will be made available and also uploaded on our website. No queries will be entertained after the Pre-bid meeting.**
5. Supply means: “Supply, Installation, Commissioning and satisfactory demonstration of the whole system and training”. If any charges extra are payable for Installation, Commissioning and training, the same should be specified in the commercial offer.
6. **Submission of Bids:**
 - (i) **Place: Purchase Section of IISER, Pune - 411 008, India.**
 - (ii) **Pre-bid Conference –11.00AM to 12.00 PM on 30.06.2016**
 - (iii) **Time and Date of Submission: Before 3.00 PM on 20.07.2016**
 - (iv) **Time and Date of opening Technical Bid: At 03.30 PM on 20.07.2016**

IISER, Pune will not be responsible, for submission / delivery of quotation at wrong places other than the Purchase Section of IISER, Pune - 411 008, India

8. Two Bid System:

The two bid system should be followed for this tender. In this system the BIDDER must submit his offer in **two separate sealed envelopes**. Both the technical bid and commercial bid envelopes should be securely sealed and stamped separately and clearly marked as **“Envelope No.1 – Technical Bid”** and **“Envelope No.2 – Commercial Bid”** respectively. Both the sealed envelopes should be placed in a third larger envelope. The main envelope which will contain both the bids should be super scribed with our **tender enquiry IISER-PUR-0225-16 due on 20.07.2016** and to be submitted to the address given below so as to reach on or before **03.00 PM on 20.07.2016**

**The Director,
Indian Institute of Science Education and Research (IISER)
Dr. Homi Bhabha Road,
Pashan,
Pune – 411 008, India**

The envelopes must be super-scribed with the following information:

- Tender Reference Number
- Due Date
- Name of the Vendor

- **Envelope No. 1 : Shall contain “Technical Bid” and Earnest Money Deposit (EMD)**

The technical offer **should not contain any price information.**

The Technical Bid must be submitted in an organized and structured manner. No brochures/leaflets etc. should be submitted in loose form. Please indicate page nos. on your quotation eg. If the quotation is containing 25 Pages, please indicate as 1/25, 2/25, 3/25 -----25/25.

The Technical Offer should comprise of the following:

- (i) The technical bid should contain commercial terms with reference to the tender.
- (iii) The technical offer should be complete to indicate that all products and services asked for are quoted. Each page of the bid and cutting/corrections shall be duly signed and stamped by the BIDDER. **Unsigned Tenders will also be rejected.** Failure to comply with this requirement may result in the bid being rejected.
- (iv) The purpose of certain specific conditions is to get or procure best Equipment/service etc. for IISER, Pune. The opinion of Technical Committee shall be the guiding factor for technical short listing.

- (vii) Undertaking that the successful BIDDER agrees to give a security deposit amounting to 10% of the purchase order value by way of Demand Draft in favor of The Director, IISER Pune.
- (viii) Duly filled in technical bid with proper seal and signature of authorized person on each page of the bid should be submitted and the same should accompany with complete specifications, Manufacturer's name, address and relevant Technical Literature/Brochures with warranty Terms and EMD.
- (ix) If the bid is for branded makes, authorization letter from principals clearly indicating that the vendor is the competent authority to sell and provide services towards the items mentioned in the scope of supply given in this tender document.
- (x) **User List :**
 - a) The list of users specifically for the same model/make of the quoted item (not the list of general users) along with the complete name, address & contact numbers of the user organizations/persons may be submitted with the quotation along with the performance certificates from all/some of them.
 - b) If you have supplied identical or similar equipment to other IISERs/IITs /CSIR Labs/Institutes., the details of such supplies for the preceding three years shall be given together with the prices finally paid. Indicate the names of the Indian reputed Organizations where you have supplied similar equipment and may attach the satisfactory performance report of the equipment from user Organization.
- (xi) Solvency certificates (not older than twelve months) issued by Scheduled/ Nationalized bank with which BIDDER holds the current account.
- (xii) Copy of LST/CST/WCT No. PAN No. and TIN No. allotted by the concerned authorities. If registered with the National Small Industries Corporation, the registration number, purpose of registration and the validity period of registration and a copy of DGS&D registration wherever it is applicable should also be provided in Technical Bid.
- (xiii) The prices should be shown against each item for the purpose of Insurance claims / replacements if any.
- (xiv) List of deliverables / Bill of materials and services.
- (xv) In case of Foreign quote, the address of Principal's / Manufacturer's and their Banker's details should be furnished.
- (xvii) The item should be supplied with manuals and the manuals including technical drawings should be complete in all respects to operate the system without any problem.

9. Specifications

Specifications are basic essence of the product. It must be ensured that the offers must be strictly as per our specifications. At the same time it must be kept in mind that merely copying our specifications in the quotation shall not make the parties eligible for consideration of the quotation. A quotation has to be supported with the printed technical leaflet/literature of the quoted model of the item by the quoting party/manufacturer and the specifications mentioned in the quotation must be reflected/supported by the printed technical leaflet/literature. Therefore the model quoted invariably be highlighted in the leaflet/literature enclosed with the quotation. Non-compliance of the above shall be treated as incomplete/ambiguous and the offer can be ignored without giving an opportunity for clarification/negotiation etc. to the quoting party

10. Compliance Statements:

- a) Bidders must furnish a Compliance Statement of each and every required Specification of our tender in the format at ANNEXURE-‘B’. The deviations, if any, from the tendered specifications should be clearly brought out in the statement. Technical literature/leaflet showing the compliance of the specification may also be attached with the quotation.
- b) Similarly, the Compliance Statement/questionnaire for Terms & Conditions of the tender may be furnished, as per the enclosed format at Annexure –‘A’, along with quotation (with techno- commercial bid in case of two bid tender system).
- c) The firms are advised to submit both the compliance statements essentially along with their quotation failing which their offer may not be considered.

Bid documents should be submitted as per the above sequence with Index page and page numbers (including technical literature). Each page of the bid should be signed & stamped in original. Unsigned bids will not be considered for evaluation.

➤ Envelope 2 : “Commercial Bid” shall contain:

- (i) Price schedule complete in all respects with proper seal and signature of authorized person. It should also contain the Comprehensive AMC charges for post warranty period as per the terms of the tender. The optional and any other essential items / accessories required for the maintenance of the equipment for the next seven years should also be specified in the offer separately. Discount offered should be mentioned clearly in the commercial bid only.



- (ii) Cost of all the items should be mentioned clearly and individually in the Commercial Offer (Part-II) only.
- (iii) The BIDDERS are requested to quote for Educational Institutional Price for Equipment and software, since we are eligible for the same.

11. Date of opening the Technical Bids.

Technical Bids will be opened on – 20.07.2016 at 03.30 PM at:

**Indian Institute of Science Education and Research (IISER)
Dr. Homi Bhabha Road, Pashan
Pune – 411 008, India**

The Technical bids will be opened in the presence of the BIDDERS on the specified time and date. BIDDERS/Agents who have responded to the tender only will be allowed to be present.

The technical bids will be evaluated to shortlist the eligible BIDDERS. The commercial bids of only the short listed BIDDERS shall be considered for further processing.

BIDDERS whose technical offer is found acceptable and meeting the eligibility requirements as specified in this tender will be informed about the date and time of the opening of the commercial bid.

Note: (i) Please do not insert 'Commercial Bid' (prices quoted) in the technical bid envelope. If the price quoted is submitted with technical bid the tender will be rejected.

(ii) No camera mobiles / mobiles are allowed during tender opening.

(iii) The bid can be submitted in person or through post/courier (IISER will not be responsible for delayed / late quotations submitted / sent by Post / Courier etc. resulting in disqualification/ rejection of any bid) so as to reach IISER on or before the due date and time. Fax / E-mail tenders will not be considered unless it is asked for. The BIDDERS' authorized representative can attend the bid opening.

(iv) No request for extension of due date will be considered under any circumstances.

(v) No sub-contracting is allowed with regard to installation, commissioning, training, warranty maintenance and after sales service. This is the sole responsibility of the Principals'/their authorized agents

12. Formation of Technical Evaluation Committee

The Technical Evaluation Committee(s) will be constituted by Director, IISER, Pune. He may nominate some external expert members, in the interest of IISER, Pune.

13. Terms of the Technical Committee

- (i) On the due date the Technical bids will be opened and referred to the Technical Committee which is duly constituted by the Director, IISER, Pune. The committee will go through the technical aspects of the tender and recommend short listed firms. The recommendation of the technical committee is the final and binding on all the parties.
- (ii) The technical evaluation will be an assessment of the Technical Bid. IISER, Pune representatives will proceed through a detailed evaluation of the Technical Bids as defined in **Chapter IV (Schedule of requirements, specifications and allied technical details)**, in order to determine whether they are substantially responsive to the requirements set forth in the tender. In order to reach such a determination, IISER, Pune will examine the information supplied by the BIDDERS, and shall evaluate the same as per the specifications mentioned in this tender.
- (iii) The technical committee may formulate evaluation criteria in addition to the specifications and requirements indicated in the tender, in the interest of IISER, Pune and this criteria/recommendation will also form as a part of short-listing of the firms.
- (iv) The Technical Committee will examine all the Technical aspects of the bids received. Further, the Technical Committee may seek additional information from the existing users at IISER, Pune or from other Institutes and also call for Technical presentations from the BIDDERS if it is required so.
- (vi) The information received and the bids already submitted together will be examined with reference to the tendered specifications and evaluation is made by the Technical Committee.
- (vii) After the technical evaluation is completed and approved, IISER, Pune shall inform to the BIDDERS whose bids have been rejected technically with the reasons for rejection.

The commercial offers of the vendors whose technical offers are found to be technically deficient or do not meet the qualification criteria as specified in this tender will be returned to them without opening along with their EMD.

- (viii) The successful BIDDERS will be informed regarding the date and time of Commercial bid opening

- (ix) The purpose of obtaining two bids (technical and commercial) is to evaluate all the firms on technical basis with reference to the tendered specifications, performance of similar Solutions/Applications elsewhere, obtaining users views with reference to the earlier supplies. This will enable the technical committee to arrive at a fair recommendation in the interest of the organization.
- (x) In the event of seeking any clarification from various BIDDERS by IISER, Pune, the BIDDERS are required to furnish only technical clarifications that are asked for. No amendment to commercial bid will be entertained at that stage. In case if a BIDDER fails to quote for a particular item it amounts to non-compliance and hence such bid will not be considered for further evaluation. Further during this process if any BIDDER indicates the price during the clarification such bids also will not be considered for further evaluation.

14. Opening of Commercial Bids

- (i) IISER will open commercial bids of only the short listed BIDDERS, in the presence of the BIDDERS or their authorized representatives who choose to attend the commercial bid opening. The Date and Time of opening the Commercial Bid will be intimated only to pre-qualified and technically acceptable BIDDERS for the item at a later date. The representatives of short listed firms only will be allowed for commercial bid opening.
- (ii) The BIDDER's representative who is present shall sign an attendance register as a proof of having attended commercial bid opening.
- (iii) The BIDDER's name, bid prices, discounts, EMD and such other details considered as appropriate by IISER, will be announced at the time of opening.

14. EVALUATION OF BIDS:

- a) IISER Pune shall correct arithmetical errors on the following basis:
 - (i) If there is a discrepancy between the unit price and the line item total that is obtained by multiplying the unit price by the quantity, the unit price shall prevail and the line item total shall be corrected, unless in the opinion of the Purchaser there is an obvious misplacement of the decimal point in the unit price, in which case the line item total as quoted shall govern and the unit price shall be corrected.
 - (ii) If there is an error in a total corresponding to the addition or subtraction of subtotals, the subtotals shall prevail and the total shall be corrected; and
 - (iii) If there is a discrepancy between words & figures, the amount in words shall prevail, unless the amount expressed in words is related to an arithmetic error, in which case the amount in figures shall prevail subject to (i) and (ii) above.

- b) Selling exchange rate/equivalent to Indian currency will be as on the date of bid opening in the case of single bidding and the rate on the date of opening of the priced bids in the case of two-part bidding.
 - c) **The bids shall be evaluated on the basis of final landing cost as per format given in Price Schedule in case of import / indigenous items.**
 - d) The comparison between the indigenous and the foreign offers shall be made on FOR destination basis and CIF/CIP basis respectively. However the CIF/CIP prices quoted by any foreign bidders shall be loaded further as under :
 - Towards customs duty and other statutory levies-as per applicable rates.
 - Towards custom clearance, inland transportation etc. – 2% of the CIF/CIP value.
 - e) Where the price quoted on FOB/FCA and CIF/CIP basis are the same, the Contract would be made on CIF/CIP basis only.
 - f) The Vague terms like “packing, forwarding, transportation..... etc. extra” without mentioning the specific amount/percentage of these charges will not be accepted. **Such offers shall be treated as incomplete and rejected.**
 - g) After arriving at final pricing of individual offers of all the short listed firms, the lowest firm will be awarded with Contract/Purchase Order.
16. The Director, IISER, PUNE reserves the right to accept the offer in full or in parts or reject summarily or partly.

CHAPTER-2 : INSTRUCTIONS TO BIDDERS

1. PREPARATION AND SUBMISSION OF OFFERS:

a) Quotation should be submitted directly by the original manufacturer/supplier or its sole authorized distributor/dealer/Indian Agent. In case of bid by authorized dealer/distributor/Indian Agent, the manufacturer authorization should be attached with the technical bid as per **Annexure-‘D’**.

One Indian Agent can participate in a tender on behalf of one manufacturer only. No offer will be entertained if the same Indian Agent is representing another manufacturer for the same item.

b) In case a bidder is not doing business within India, it shall furnish the certificate to the effect that the bidder is or will be represented by an agent in India equipped and able to carry out the supply, maintenance, repair obligations etc. during the warranty and post-warranty period or ensure a mechanism at place for carrying out the supply, maintenance, repair obligations etc. during the warranty and post-warranty period.

c) The bidder shall bear all costs associated with the preparation and submission of its bid irrespective of the conduct or outcome of the bidding process.

d) The bidder should not indulge in any corrupt, fraudulent, collusive, coercive practices during the entire process of procurement and execution of contract/order.

e) Before the deadline for submission of the bid, IISER PUNE reserves the right to modify the bidding document and to extend or not to extend the date of submission. Such amendment/modification will be hosted on IISER PUNE website.

d) Conditional tenders will be summarily rejected.

e) A bidder may withdraw, substitute, or modify its bid after it has been submitted by sending a written notice signed by the authorized signatory before the date of submission of the bid. Any re-submission or modification in the bid should be submitted before the date & time of submission of bid as originally conveyed in the invitation of bid.

f) No bid may be withdrawn, substituted or modified in the interval between the deadline for submission of bids and the expiration of the period of bid validity specified by the Bidder on the Bid Form or any extension thereof.

In case of above, first envelope marked “WITHDRAWAL” shall not be opened, but returned to the Bidder subject to submission of valid authorization to request the withdrawal. In case of substituted and modified bid, only the substituted bids and modified bids will be opened subject to production of authorization from the bidders.

The offers must contain the following documents :-

(A) Techno-commercial offers must contain:

- (i) Manufacturer authorization as per **Annexure –‘D’**.
- (ii) Certificate by bidder not doing business in India.

- (iii) Technical literature/ leaflets and complete specifications of quoted model(s) along with commercial terms and conditions.
- (iv) Compliance statement/questionnaire of tender terms and conditions as per **Annexure-‘A’**
- (v) Compliance statement of specifications as per **Annexure- ‘B’**
- (vi) Bid Security/EMD as per **Annexure- ‘C’**
- (vii) In case of exemption from submission of Bid security, proof of registration with DGS&D/NSIC .
- (viii) Copies of previous supply orders as per **Annexure –‘E’**.
- (ix) Details of supplies of similar equipments .

2. Delivery Period / Timeliness

- 2.1 The deliveries & installation must be completed **within 2 month** after placement of purchase order. The time is the essence of the contract. It is mandatory for the BIDDERS who respond to this bid to meet these expectations, as are tightly linked to IISER, PUNE's plans of completing the project within the time frame.

3. Earnest Money Deposit (EMD)

- 3.1 The tender documents must be accompanied by Earnest Money Deposit (**EMD**) of **Rs 62,000/- (Rs Sixty Two Thousand only)** EMD in the form of Bank guarantee (As per format enclosed as ANNEXURE- ‘C’) or Demand Draft of a scheduled bank in the name of Director, IISER, Pune valid for 180 days from the date of opening of the tender. The firm registered with DGS&D/NSIC as manufacturer for the supply of the same category of item for which the party is submitting quotation will be exempted from submission of EMD. Intended parties will have to give proof of registration along with their quotation. EMD of the unsuccessful bidders shall be refunded without any interest at the earliest after finalization of the purchase of concerned item. The party must therefore, submit a pre-receipted Bill in triplicate along with the quotation (in case of EMD sent in form of Bank Draft) to enable us to refund their EMD.
- 3.2 The BIDDER who submits the tender on behalf of their principals should produce documentary evidence in support of their authority to quote or submit proforma invoice of their principals. In case the BIDDER is not represented by any Indian Agent the Bank Guarantee valuing **US \$ 950.00 (US Dollars Nine Hundred and Fifty only)** should accompany the Technical Bid towards EMD.
- 3.3 In case of bids in Foreign Currency, the Indian Representative / dealers can submit the EMD in INR to IISER, Pune without any relaxation.
- 3.4 The Bank Guarantee is insisted due to steep fluctuations in foreign exchange hence the foreign DD's are not accepted towards EMD.

- 3.5 Bids submitted without EMD will stand rejected. EMD will not be accepted in the form of cash / cheque . No interest is payable on EMD.
- 3.6 The EMD will be returned to the BIDDERS(s)/Agents whose offer is not accepted by IISER, PUNE within one month from the date of the placing of the final order(s) on the selected BIDDER(s). In case of the BIDDER(s) whose offer is accepted the EMD will be returned on submission of Bank Guarantee as Security Deposit (SD). However, if the return of EMD is delayed for any reason, no interest / penalty shall be payable to the BIDDERS.
- 3.7 **The successful BIDDER, on award of contract / order, must send the contract / order acceptance in writing, within 15 days of award of contract / order failing which the EMD will be forfeited.**
- 3.8 The EMD shall be forfeited:
 - 3.8.1 If the BIDDER withdraws the bid during the period of bid validity specified in the tender.
 - 3.8.2 In case a successful BIDDER fails to furnish the Security Deposit.
4. **Security Deposit**
 - 4.1 Within ten (15) days of the award of contract, the vendor shall furnish a Security Deposit amounting to 10% of the purchase order value in the form of Demand Draft/Bank Guarantee **(from scheduled Bank only)** favoring the Director, Indian Institute of Science Education and Research, Pune.
 - 4.2 The IISER will forfeit the 10% security deposit if vendor fails to execute the order as per the Purchase Order. This Security Deposit will be refunded to the vendor only on successful installation of the EQUIPMENT / SYSTEM.
 - 4.3 The Security Deposit should be valid for a period of warranty period as we plan to extend the same as Performance Bank Guarantee.
 - 4.4 **Bank Guarantee wherever mentioned in this document may be read as “Bank Guarantee from any Scheduled Bank” only.**
5. **Amalgamation/Acquisition etc.:**

In the event the Manufacturer/Supplier proposes for amalgamation, acquisition or sale of its business to any firm during the contract period, the BUYER/Successor of the Principal Company are liable for execution of the contract and also fulfillment of contractual obligations i.e.supply, installation,



commissioning, warranty, maintenance/replacement of spares accessories etc. while submitting your bid, you may confirm this condition.

6. **Period of validity of bids**

- 6.1. The prices must be valid at least for a period of **90 days for indigenous supplies & 180 days for imports** from the date of opening of the Tender. No changes in prices will be acceptable in any condition after opening of tender till the validity of the offer or execution of the order whichever is later
- 6.2. IISER, PUNE may ask for the BIDDER's consent to extend the period of validity. Such request and the response shall be made in writing only. The BIDDER is free not to accept such request without forfeiting the EMD. A BIDDER agreeing to the request for extension will not be permitted to modify his bid.
- 6.3 Bid evaluation will be based on the bid prices without taking into consideration the above corrections.

SUBMISSION OF BIDS

7. **Deadline for submission of Bids**

- 7.1 Bids must be received by IISER, PUNE **before the time & date at address specified in the tender.** In the event of specified date for the submission of bids being declared as a holiday for IISER, PUNE, the bid-closing deadline will stand extended to the next working day. No communication is required in such cases, In the event of holiday on due date
- 7.2 IISER, PUNE may, extend this deadline for submission of bids, this will suitably be notified on the IISER, PUNE website.

8. **Late Bids**

IISER, PUNE will not be responsible:

- 8.1 For delayed / late quotations submitted / sent by post / courier etc.
- 8.2 For submission / delivery of quotations at wrong places other than the Purchase section of IISER, Pune.
- 8.3 Fax / E-mail / Telegraphic / Telex tenders will not be considered.
- 8.4 Any bid inadvertently received by IISER, PUNE after the deadline i.e. due date & time for submission of bids, will not be accepted and returned unopened to the BIDDER.



AWARD OF CONTRACT

9. Award Criteria

- 9.1 IISER, PUNE shall award the contract to the technically qualified eligible BIDDER whose bid has been determined as the lowest evaluated commercial bid.
- 9.2 If more than one BIDDER happens to quote the same lowest price, IISER, PUNE reserves the right to award the contract to more than one BIDDER or any BIDDER.

10. IISER Pune Right to vary Quantities at the time of Award

- 10.1. The IISER Pune reserves the right at the time of Contract award to increase or decrease the quantity of goods and services originally specified in the tender document without any change in unit price or other terms and conditions. Further, at the discretion of the IISER Pune, the quantities in the contract may be enhanced by 30% within the delivery period.
- 10.2. Firms which have already supplied similar equipment to IISER, PUNE and have not completed required installation/commissioning/after sales service/warranty replacements etc. such firms offers will not be considered for further evaluation and no enquiries thereafter will be entertained.

11. Cargo Consolidation and Customs Clearance:

IISER, PUNE has appointed its own Freight Forwarder and Custom House Agent for all IISER, imports. Please note that all the consignments have to be routed through their associates only. The address and contact details will be provided at the time of placing the Purchase Order. While submitting your bid, you may confirm this condition.

12. Fraud and Corruption

The IISER Pune requires that bidders, suppliers, contractors and consultants, if any, observe the highest standard of ethics during the procurement and execution of such contracts. In pursuit of this policy,

- (a) The terms set forth below are defined as follows:
 - (i) **“Corrupt practice”** means the offering, giving, receiving, or soliciting, directly or in indirectly, of anything of value to influence the

action of a public official in the procurement process or in contract execution;

- (ii) **“Fraudulent practice”** means a misrepresentation or omission of facts in order to influence a procurement process or the execution of a contract;
- (iii) **“Collusive practice”** means a scheme or arrangement between two or more bidders, designed to establish bid prices at artificial, noncompetitive levels; and
- (iv) **“Coercive practice”** means harming or threatening to harm, directly or indirectly, persons or their property to influence their participation in the procurement process or affect the execution of a contract;

- (b) The IISER Pune will reject a proposal for award if it determines that the Bidder recommended for award has, directly or through an agent, engaged in corrupt, fraudulent, collusive or coercive practices in competing for the Contract in question;

13. Interpretation of the clauses in the Tender Document / Contract Document

In case of any ambiguity / dispute in the interpretation of any of the clauses in this Tender Document, **Director, IISER, PUNE’s interpretation of the clauses shall be final and binding on all parties.**

CHAPTER - 3 : CONDITIONS OF CONTRACT

1. Prices

Bid prices should be filled in the appropriate format as mentioned in Price Schedule.

ALL THE BIDDERS SHOULD QUOTE PRICES FOR EACH AND EVERY ITEM SEPERATELY ALONG WITH THE CONSOLIDATED PRICES APPLICABLE FOR BOTH INDIGENOUS AND IMPORTED ITEMS.

A. For Goods manufactured in India:

- (i) The price of goods quoted Ex-Works including taxes already paid.
- (ii) VAT and other taxes like excise duty etc. which will be payable on the goods if the contract is awarded.
 - (a) The charges for inland transportation, insurance and other local service required for delivering the goods at the desired destination as specified in the price schedule form.
 - (b) The installation, commissioning and training charges including any incidental services, if any.

B. For Goods manufactured abroad:

- (i) The price of the goods, quoted on FCA (Named place of delivery abroad) or FOB (Named port of shipment), as specified in the schedule form.
- (ii) The charges for insurance and transportation of the goods to the port/place of destination.
- (iii) The agency commission charges, if any.
- (iv) The installation, commissioning and training charges including any incidental services, if any.

C. We are exempted from payment of Excise Duty under notification number 10/97 dated 01.03.1997 and Customs Duty under notification No.51/96 dated 23.07.1996. **Hence Excise Duty and Customs Duty, if any, should be shown separately. No other charges than those mentioned clearly in the quotation will be paid.**

D. Sales Tax: We are not authorized to issue any Sales Tax Form 'C' & 'D'.

E. BIDDERS may also bid for High Sea sales.

2. Bank Charges

All Bank charges inside India, including opening of LC, to IISER, PUNE Account and outside India to Beneficiary's Account only. In case the BIDDER seeks confirmation of LC such confirmation charges are to the Beneficiary's account. This may please be noted and confirmed.

3. **Agency Commission & Services**

- 3.1. The Indian Agency commission payable in Indian currency only after the receipt of consignment in good condition at our Stores and satisfactory installation and commissioning of the ordered equipment.
- 3.2. In case of foreign quote, the Principal supplier should clearly indicate the address of the Indian Agent and percentage (%) of Agency Commission and taxes if any payable to him. Such amounts will be paid in Indian Currency to the Indian Agent.
- 3.3. Details of services rendered by you as well as after-sales services offered by you are to be made clear in the tender.

7. **Performance Bank Guarantee**

The 10% Security Deposit which is mentioned above may be extended as Performance Bank Guarantee for a period of warranty period.

8. **Performance Benchmarks**

The technical evaluation committee needs to be provided with an evaluation system to carry out performance benchmarks.

9. **Pre-installation:**

The BIDDER has to state in detail the Electrical Power/UPS requirements, floor Space, head room, foundation needed and also to state whether Air-conditioned environment is needed to house the system and to run the tests. i.e. pre-installation facilities required for installation may please be intimated in the technical bid. Subsequently, before the consignment lands in IISER, Pune the BIDDER shall confirm that the pre-installation requirements are sufficient for installation of the equipment. In other words the BIDDER should continuously monitor the pre-installation requirements and see that everything is ready before the consignment is taken to the site for installation.

10. **INSTALLATION**

- 10.1 BIDDER shall be responsible for installation / demonstration wherever applicable and for after sales service during the warranty and thereafter.
- 10.2. Installation demonstration to be arranged by the supplier free of cost and the same is to be done within 15 days of the arrival of the equipment at site.
- 10.3. After successful installation what will be the minimum down time of equipment/instrument in case of breakdown. If the identified firm or person fails to put the system into working condition what is the

further alternative course of action suggested by you to adhere to minimum down time.

11. **INSPECTION** :

- 11.1 The inspection of the system will be done by our technical expert /Scientist in the presence of firm's representative.
- 11.2 In case of receipt of the material in short supply or damaged condition the supplier will have to arrange the supplies/ replacement of goods free of cost pending the settlement of the insurance case wherever applicable on FOR at the IISER. Or CIF basis till satisfactory installation of the system.
- 11.3 The supplier **should arrange for physical inspection of the items directly or through their authorized representative within seven days of arrival of the consignment failing which they will be responsible for the losses.** After the shipment is effected, the supplier/its representative/Indian agents must remain in touch with the lab/instit. to ascertain the date of arrival of consignment.

12. **Training**

- 12.1 Wherever needed, Our Scientist/Technical persons should be trained by the supplier at the project site free of cost. In case the person is to be trained at supplier's site abroad or in India it should be mentioned in the quotation clearly. The supplier should bear all the expenses for such training including 'to & fro' fares and lodging & boarding charges.

13. **Warranty / Support**

- 13.1. The items covered by the schedule of requirement shall carry minimum **three years of comprehensive warranty** from the date of acceptance of the equipment by IISER, PUNE. Warranty shall include free maintenance of the whole equipment supplied including free replacement of parts. The defects, if any, shall be attended to on immediate basis but in no case any defect should prolong for more than 24 hours. The comprehensive warranty includes onsite warranty with parts.
- 13.2. The defects, if any, during the guarantee/warranty period are to be rectified free of charge by arranging free replacement wherever necessary. This includes cost, insurance, freight, custom duty, octroi, local taxes if any should be borne by the beneficiary or his agent. A clear confirmation should be given for this item.

- 13.3. The warranty on the associated software should cover providing of upgraded version/s, if any, released during the warranty period free of cost.
 - 13.4. The BIDDER shall assure the supply of spare parts after warranty is over for maintenance of the equipment supplied if and when required for a period of 10 years from the date of supply of equipment on payment on approved price list basis.
 - 13.5. The equipment must be supported by a Service Centre in India manned by the principal vendor's technical support engineers. The support through this Centre must be available 24 hours in a day, seven days a week and 365 days a year. Also it should be possible to contract the Principal's vendor support Centre on a toll free number/web/mail.
 - 13.6. An undertaking from the manufacturer is required in this regard stating that they would facilitate the BIDDER on regular basis with technology / product updates & extend support for the warranty as well.
 - 13.7. The vendor will have to arrange for all the testing equipment & tools required for installation, testing & maintenance etc.
 - 13.8. The principal vendor must have a local logistics support by maintaining a local spares depot in the country of deployment of the equipment. This is to ensure immediate delivery of spares parts from Principal Vendor of equipment to its channel partner/system integrator.
 - 13.9. Details of onsite warranty, agency who shall maintain during warranty and undertake Annual Maintenance Contract/Comprehensive Service Maintenance Contract beyond warranty shall be given in the offer. In case of foreign quote, the Indian Agent who shall maintain during warranty and AMC beyond warranty shall be given in the Technical Offer.
 - 13.10 **COMMENCEMENT OF WARRANTY PERIOD:** The warranty period of an item shall commence after receipt of the items in good working condition and from the date of its satisfactory installation/commissioning/demonstration at the project site in IISER,, Pune. The warranty period and validity of Performance Guarantee shall be extended for the period of delay in satisfactory installation and delay in warranty service.
14. **Reasonability of Prices:**
- 14.1. Please quote best minimum prices applicable for a premiere Educational and Research Institution,
 - 14.2. The party must give details of identical or similar equipment, if any, supplied to any IITS/IISERS/ CSIR lab during last three years along with the final price paid and Performance certificate from them.

15. Annual Maintenance Contract

- 15.1. The party must mention in the quotation, the rate/amount of annual maintenance charges, if we opt for maintenance contract after expiry of the warranty period. This is mandatory to mention, wherever applicable.
- 15.2. No sub-contracting will be allowed for installation or maintaining system/ equipment / instrument during or after warranty period.

16. Indemnity

The vendor shall indemnify, protect and save IISER, PUNE against all claims, losses, costs, damages, expenses, action suits and other proceeding, resulting from infringement of any law pertaining to patent, trademarks, copyrights etc. or such other statutory infringements in respect of all the equipments supplied by him.

17. Freight & Insurance

- 17.1. Imports: In case of imports the freight & insurance will be paid by IISER, PUNE, as the consignments are shipped through the IISER, PUNE nominated freight forwarder (applicable only cases of FCA/FOB shipments) .
- 17.2. Indigenous : The equipments to be supplied will be insured by the vendor against all risks of loss or damage from the date of shipment till such time it is delivered at IISER, PUNE site in case of Rupee transaction.

18. Payment

- 18.1. For Indigenous items, 90% payment shall be made against delivery, installation, commissioning and on acceptance as per Purchase Order at site and balance 10% shall be made after receipt of performance Bank Guarantee for 10% of the total order value, to be valid for till warranty period from date of installation and acceptance. If no Bank Guarantee is given, the balance 10% will be paid after assessing, after sales service during warranty period i.e. payment after warranty period.
- 18.2. For imported items, 90% payment shall be made by a Irrevocable Letter of Credit established in favor of the supplier through the State Bank of India, Deccan Gymkhana Branch, Pune 411 004 (India) for the order value, excluding the Agency Commission due to the Indian Agents, against the presentation of original Shipping documents. Balance 10% will be released after completion of satisfactory installation, commissioning, demonstration of the whole system, after imparting training and upon receipt of Bank Guarantee for 10% of

total Order value towards performance security to be valid for till warranty period from the date of installation. However Letter of Credit arrangement will be made for 100% order value.

The payment of local currency portion shall be payable in equivalent Indian Rupees, within 30 days after the receipt of the equipment in good condition and after satisfactory installation and commissioning and demonstration.

The Agency Commission to the Indian Agent will be paid in INR only after successful installation, commissioning and satisfactory demonstration and acceptance of the items ordered for by the end user.

19. Penalty for delayed Services / LD

- 19.1. As time is the essence of the contract, Delivery period mentioned in the Purchase Order should be strictly adhered to. Otherwise the IISER will forfeit EMD/SD and also LD clause will be applicable /enforced.
- 19.2. If the supplier fails to Supply, Install and Commission the system as per specifications mentioned in the order within the due date, the Supplier is liable to pay liquidated damages of 1% of order value per every week of delay subject to a maximum of 10% beyond the due date. Such money will be deducted from any amount due or which may become due to the supplier.
- 19.3. IISER, PUNE reserves the right to cancel the order in case the delay is more than 10 weeks. Penalties, if any, will be deducted from the Security Deposit.

20. Jurisdiction

The disputes, legal matters, court matters, if any, shall be subject to Pune Jurisdiction only.

21. Force Majeure

The Supplier shall not be liable for forfeiture of its performance bank guarantee, liquidated damages or termination for default, if and to the extent that, it's delay in performance or other failure to perform its obligations under the Contract is the result of an event of Force Majeure. For purposes of this Clause, "Force Majeure" means an event beyond the control of the Supplier and not involving the Supplier's fault or negligence and not foreseeable. Such events may include, but are not limited to, acts of the IISER Pune either in its sovereign or contractual capacity, wars or revolutions, fires, floods, epidemics, quarantine restrictions and freight embargoes.

If a Force Majeure situation arises, the Supplier shall promptly notify the IISER Pune in writing of such conditions and the cause thereof. Unless otherwise directed by the IISER Pune in writing, the Supplier shall continue to perform its obligations under the contract as far as is reasonably practical, and shall seek all reasonable alternative means for performance not prevented by the Force Majeure event.

22. Dispute Settlement

IISER Pune and the Supplier shall make every effort to resolve amicably by direct informal negotiation any disagreement or dispute arising between them under or in connection with the Contract.

If, after twenty-one (21) days, the parties have failed to resolve their dispute or difference by such mutual consultation, then either the IISER Pune or the Supplier may give notice to the other party of its intention to commence arbitration, as hereinafter provided, as to the matter in dispute, and no arbitration in respect of this matter may be commenced unless such notice is given. Any dispute or difference in respect of which a notice of intention to commence arbitration has been given in accordance with this Clause shall be finally settled by arbitration. Arbitration may be commenced prior to or after delivery of the Goods under the Contract.

The dispute settlement mechanism/arbitration proceedings shall be concluded as under:

- (a) In case of Dispute or difference arising between the IISER Pune and a domestic supplier relating to any matter arising out of or connected with this agreement, such disputes or difference shall be settled in accordance with the Indian Arbitration & Conciliation Act, 1996, the rules there under and any statutory modifications or re-enactments thereof shall apply to the arbitration proceedings. The dispute shall be referred to the Director IISER Pune, if he is unable/unwilling to act, to the sole arbitration of some other person appointed by his willing to act as such Arbitrator. The award of the arbitrator so appointed shall be final, conclusive and binding on all parties to this order.
- (b) In the case of a dispute between the Purchase and a Foreign supplier, the dispute shall be settled by arbitration in accordance with provision of sub-clause (a) above. But if this is not acceptable to the supplier then the dispute shall be settled in accordance with provisions of UNCITRAL (United Nations Commission on International Trade Law) Arbitration Rules.

The venue of the arbitration shall be the place from where the purchase order or contract is issued.

CHAPTER 4

SCHEDULE OF REQUIREMENTS, SPECIFICATIONS & ALLIED TECHNICAL DETAILS

Specifications for

IISRE PUNE : AIR SHOWER AND GARMENT CABINET SPECIFICATIONS

TECHNICAL SPECIFICATIONS FOR AIR SHOWER AT MAIN ENTRY AT GROUND FLOOR

1.	ITEM	AIR SHOWER
2.	MOC	OUTER SIDE CRCA POWDER COATED, INNER SIDE SS 304, MATT FINISH COLOUR-RAL 9002 (OFFWHITE)
3.	CLASS	100
4.	QUANTITY	01 NO.
5.	SIZE	OVERALL DIM : 2400 (W) X 3100 (D) X 2150 (H) MM WORKSPACE DIM : 1500 (W) X 3040 (D) X 2050 (H) MM
6.	SUPPLY FILTER	MINIPLEAT HEPA AIR FILTER EFFICIENCY : 99.997% DOWN TO 0.3 MICRON GRADE : H - 14 MEDIA : MICRO GLASS FIBRE PAPER (IMPORTED) INITIAL P.D. : 15 MM OF W.G. FINAL P.D. : 40 MM OF W.G. SEPERATOR : HOT MELT GLOVE SEALING : EPOXY BASED PU ADHESIVE CASING : FACTORY EXTRUDED AL. SECTION, BOX TYPE SIZE : 610 (W) X 610 (H) X 100 (D) MM – 04 NOS.
7.	PRE FILTER	PRE FILTER FOR SECONDARY SUCTION GRADE : F7 GRADE AS PER BSEN 779 INITIAL P.D. : 6.5 MM OF W.G. FINAL P.D. : 13.0 MM OF W.G. SEPERATOR : ALUMINIUM SEALING : EPOXY BASED PU ADHESIVE CASING : ALUMINIUM ANODISED FLANGE TYPE SIZE : FLANGE - 690 X 390 BOX - 625 X 320 X 50 MM - 04 NOS.
8.	BLOWER MOTOR ASSEMBLY	ELECTRIC MOTOR - 1 HP, 3 PHASE, 2845 RPM, 415 V AC, 50 HZ HINDUSTAN MAKE DOUBLE SHAFT – 04 NOS. G.I. IMPELLER – 7 ½ ” X 4 ½ ”, STATISTICALLY AND DYNAMICALLY BALANCED ALUMINIUM IMPELLERS – 01 SET (L+R) BLOWER CASING – FRP BLOWER CASING WITH REXINE CONNECTOR AND ANTIVIBRATION MOUNTING
9.	AIR JET NOZZLES	RIGHT SIDE NOZZLES – 14 NOS. LEFT SIDE NOZZLES – 14 NOS. TOP SIDE PLASTIC NOZZLES – 16 NOS. (ID - Ø 28 MM, OD - Ø 125 MM) AIR VELOCITY – 30 M/SEC AT NOZZLE
10.	DOOR	MOC - SS 304 WITH HALF GLASS WINDOW, DOOR

	CLOSER, HANDLES, HINGES, INTERLOCKING SYSTEM FOR BOTH ENTRY AND EXIT DOOR. SIZE – 800 (W) X 2050 (H) X 25 MM THK.
--	---

11.	CONTROL LOGIC	<p>PROGRAMMABLE LOGIC CONTROLLER (PLC) ACTIVATING THE EMERGENCY SWITCH SHALL CAUSE THE CYCLE TO IMMEDIATELY END AND RELEASE ALL INTERLOCKS, LIGHT SHALL REMAINS ON</p> <p>NOMENCLATURE</p> <ol style="list-style-type: none"> 1. D1: ENTRY DOOR 2. D2: EXIT DOOR <p>IN NORMAL CONDITION, DOOR D1 AND D2 ARE IN UNLOCK CONDITION.</p> <p>FOR UNIT ON - MAINS ON - TUBELIGHT GETS ON BY ROTARY SWITCH</p> <p>DETAILS OF LOGIC SEQUENCE <u>FOR ONE SIDE ENTRY</u> FIRST CYCLE OF OPERATION –</p> <ol style="list-style-type: none"> 1. WHEN DOOR D1 IS OPENED DOOR D2 GETS LOCKED BLOWER IS IN OFF CONDITION 2. DOOR D1 IS CLOSED, THEN DOOR D2 GETS LOCKED AND BLOWER MOTOR GETS ON BOTH DOORS ARE LOCK 3. BLOWER MOTOR (AS PER TIMER SETTING 0-120 SEC) GETS OFF, THEN DOOR D2 GETS OPENED/UNLOCKED D1 LOCKED 4. DOOR D2 IS CLOSED DOOR D1 AND D2 GETS OPENED/UNLOCKED BLOWER GETS OFF D1 LOCK – (ONE TIME ONE DOOR OPEN - D1 OPEN – D2 LOCK D2 OPEN –D1 LOCK <p style="text-align: center;">OR</p> <p><u>FOR BOTH SIDE ENTRY</u> SAME SEQUENCE OF OPERATION IS REPEATED FOR FURTHER CYCLE OF OPERATION</p> <p>GREEN INDICATION - OPEN RED INDICATION – LOCK</p>
-----	---------------	---

12.	ELECTRICALS	<ul style="list-style-type: none"> * ON/OFF SWITCHES FOR OPERATING B/MOTOR, TUBE LIGHT AND AUXILLARY SOCKET * AUTOMATIC DOOR INTERLOCKING SYSTEM ALONG WITH ELECTROMAGNETS, TIMER, MAGNETIC STRIP, EMERGENCY RELEASE SWITCH AND DOOR INDICATOR IS PROVIDED * LIGHT – 20 W, PHILLIPS MAKE FLUROSCENT TUBE – 01 NO. * 3 CORE CONNECTION CABLE – 3 METER LONG * REQUIRED SUPPLY – 415 V, 3 PHASE, 50 HZ.
13.	FEATURES	* FLOORING – SS PERFORATION
14.	DOCUMENTATION	DESIGN QUALIFICATION OPERATIONAL QUALIFICATION INSTALLATION QUALIFICATION PERFORMANCE QUALIFICATION
15.	TEST CERTIFICATES	MOC TEST CERTIFICATE MOTOR BLOWER TEST CERTIFICATE HEPA FILTER TEST CERTIFICATE PRE FILTER TEST CERTIFICATE

TECHNICAL SPECIFICATIONS FOR AIR SHOWER AT FIRST AND SECOND FLOOR ENTRY

1.	ITEM	AIR SHOWER
2.	MOC	OUTER SIDE CRCA POWDER COATED, INNER SIDE SS 304, MATT FINISH COLOUR-RAL 9002 (OFFWHITE)
3.	CLASS	100
4.	QUANTITY	01 NO.
5.	SIZE	OVERALL DIM : 1980 (W) X 1500 (D) X 2150 (H) MM WORKSPACE DIM : 1080 (W) X 1440 (D) X 2050 (H) MM
6.	SUPPLY FILTER	MINIPLEAT HEPA AIR FILTER EFFICIENCY : 99.997% DOWN TO 0.3 MICRON GRADE : H - 14 MEDIA : MICRO GLASS FIBRE PAPER (IMPORTED) INITIAL P.D. : 15 MM OF W.G. FINAL P.D. : 40 MM OF W.G. SEPERATOR : HOT MELT GLOVE SEALING : EPOXY BASED PU ADHESIVE CASING : FACTORY EXTRUDED AL. SECTION, BOX TYPE SIZE : 610 (W) X 915 (H) X 100 (D) MM – 02 NOS.
7.	PRE FILTER	PRE FILTER FOR SECONDARY SUCTION GRADE : F7 GRADE AS PER BSEN 779 INITIAL P.D. : 6.5 MM OF W.G. FINAL P.D. : 13.0 MM OF W.G. SEPERATOR : ALUMINIUM SEALING : EPOXY BASED PU ADHESIVE CASING : ALUMINIUM ANODISED FLANGE TYPE SIZE : FLANGE - 1190 X 390 BOX - 1130 X 320 X 50 MM - 02 NOS.
8.	BLOWER MOTOR ASSEMBLY	ELECTRIC MOTOR - 1 HP, 3 PHASE, 2845 RPM, 415 V AC, 50 HZ HINDUSTAN MAKE DOUBLE SHAFT – 02 NOS. G.I. IMPELLER – 7 ½ ” X 4 ½ ”, STATISTICALLY AND DYNAMICALLY BALANCED ALUMINIUM IMPELLERS – 01 SET (L+R) BLOWER CASING – FRP BLOWER CASING WITH REXINE CONNECTOR AND ANTIVIBRATION MOUNTING
9.	AIR JET NOZZLES	RIGHT SIDE NOZZLES – 09 NOS. LEFT SIDE NOZZLES – 09 NOS. TOP SIDE PLASTIC NOZZLES – 04 NOS. (ID - Ø 28 MM, OD - Ø 125 MM) AIR VELOCITY – 30 M/SEC AT NOZZLE
10.	DOOR	MOC - SS 304 WITH HALF GLASS WINDOW, DOOR CLOSER, HANDLES, HINGES, INTERLOCKING SYSTEM FOR BOTH ENTRY AND EXIT DOOR. SIZE – 800 (W) X 2050 (H) X 25 MM THK.

11.	CONTROL LOGIC	<p>PROGRAMMABLE LOGIC CONTROLLER (PLC) ACTIVATING THE EMERGENCY SWITCH SHALL CAUSE THE CYCLE TO IMMEDIATELY END AND RELEASE ALL INTERLOCKS, LIGHT SHALL REMAINS ON</p> <p>NOMENCLATURE</p> <ol style="list-style-type: none"> 1. D1: ENTRY DOOR 2. D2: EXIT DOOR <p>IN NORMAL CONDITION, DOOR D1 AND D2 ARE IN UNLOCK CONDITION.</p> <p>FOR UNIT ON - MAINS ON - TUBELIGHT GETS ON BY ROTARY SWITCH</p> <p>DETAILS OF LOGIC SEQUENCE <u>FOR ONE SIDE ENTRY</u> FIRST CYCLE OF OPERATION –</p> <ol style="list-style-type: none"> a) WHEN DOOR D1 IS OPENED DOOR D2 GETS LOCKED BLOWER IS IN OFF CONDITION b) DOOR D1 IS CLOSED, THEN DOOR D2 GETS LOCKED AND BLOWER MOTOR GETS ON BOTH DOORS ARE LOCK c) BLOWER MOTOR (AS PER TIMER SETTING 0-120 SEC) GETS OFF, THEN DOOR D2 GETS OPENED/UNLOCKED D1 LOCKED d) DOOR D2 IS CLOSED DOOR D1 AND D2 GETS OPENED/UNLOCKED BLOWER GETS OFF D1 LOCK – (ONE TIME ONE DOOR OPEN - D1 OPEN – D2 LOCK D2 OPEN –D1 LOCK <p style="text-align: center;">OR</p> <p><u>FOR BOTH SIDE ENTRY</u> SAME SEQUENCE OF OPERATION IS REPEATED FOR FURTHER CYCLE OF OPERATION</p> <p>GREEN INDICATION - OPEN RED INDICATION – LOCK</p>
-----	---------------	---

12.	ELECTRICALS	<ul style="list-style-type: none"> * ON/OFF SWITCHES FOR OPERATING B/MOTOR, TUBE LIGHT AND AUXILLARY SOCKET * AUTOMATIC DOOR INTERLOCKING SYSTEM ALONG WITH ELECTROMAGNETS, TIMER, MAGNETIC STRIP, EMERGENCY RELEASE SWITCH AND DOOR INDICATOR IS PROVIDED * LIGHT – 20 W, PHILLIPS MAKE FLUROSCENT TUBE – 01 NO. * 3 CORE CONNECTION CABLE – 3 METER LONG * REQUIRED SUPPLY – 415 V, 3 PHASE, 50 HZ.
13.	FEATURES	* FLOORING – SS PERFORATION
14.	DOCUMENTATION	DESIGN QUALIFICATION OPERATIONAL QUALIFICATION INSTALLATION QUALIFICATION PERFORMANCE QUALIFICATION
15.	TEST CERTIFICATES	MOC TEST CERTIFICATE MOTOR BLOWER TEST CERTIFICATE HEPA FILTER TEST CERTIFICATE PRE FILTER TEST CERTIFICATE

TECHNICAL SPECIFICATIONS FOR AIR SHOWER AT SKID AND NUDE NICE LA AT FIRST AND SECOND FLOOR.

1.	ITEM	AIR SHOWER
2.	MOC	OUTER SIDE CRCA POWDER COATED, INNER SIDE SS 304, MATT FINISH COLOUR-RAL 9002 (OFFWHITE)
3.	CLASS	100
4.	QUANTITY	01 NO.
5.	SIZE	OVERALL DIM: 1500 (W) X 2000 (D) X 2150 (H) MM WORKSPACE DIM : 800 (W) X 1940 (D) X 2050 (H) MM
6.	SUPPLY FILTER	MINIPLEAT HEPA AIR FILTER EFFICIENCY : 99.997% DOWN TO 0.3 MICRON GRADE : H - 14 MEDIA : MICRO GLASS FIBRE PAPER (IMPORTED) INITIAL P.D. : 15 MM OF W.G. FINAL P.D. : 40 MM OF W.G. SEPERATOR : HOT MELT GLOVE SEALING : EPOXY BASED PU ADHESIVE CASING : FACTORY EXTRUDED AL. SECTION, BOX TYPE SIZE : 610 (W) X 610 (H) X 100 (D) MM – 02 NOS.
7.	PRE FILTER	PRE FILTER FOR SECONDARY SUCTION GRADE : F7 GRADE AS PER BSEN 779 INITIAL P.D. : 6.5 MM OF W.G. FINAL P.D. : 13.0 MM OF W.G. SEPERATOR : ALUMINIUM SEALING : EPOXY BASED PU ADHESIVE CASING : ALUMINIUM ANODISED FLANGE TYPE SIZE : FLANGE - 690 X 390 BOX - 625 X 320 X 50 MM - 02 NOS.
8.	BLOWER MOTOR ASSEMBLY	ELECTRIC MOTOR - 1 HP, 3 PHASE, 2845 RPM, 415 V AC, 50 HZ HINDUSTAN MAKE DOUBLE SHAFT – 02 NOS. G.I. IMPELLER – 7 ½ ” X 4 ½ ”, STATISTICALLY AND DYNAMICALLY BALANCED ALUMINIUM IMPELLERS – 01 SET (L+R) BLOWER CASING – FRP BLOWER CASING WITH REXINE CONNECTOR AND ANTIVIBRATION MOUNTING
9.	AIR JET NOZZLES	RIGHT SIDE NOZZLES – 14 NOS. LEFT SIDE NOZZLES – 14 NOS. TOP SIDE PLASTIC NOZZLES – 04 NOS. (ID - Ø 28 MM, OD - Ø 125 MM) AIR VELOCITY – 30 M/SEC AT NOZZLE

10.	DOOR	MOC - SS 304 WITH HALF GLASS WINDOW, DOOR CLOSER, HANDLES, HINGES, INTERLOCKING SYSTEM FOR BOTH ENTRY AND EXIT DOOR. SIZE – 800 (W) X 2050 (H) X 25 MM THK.
11.	CONTROL LOGIC	<p>PROGRAMMABLE LOGIC CONTROLLER (PLC) ACTIVATING THE EMERGENCY SWITCH SHALL CAUSE THE CYCLE TO IMMEDIATELY END AND RELEASE ALL INTERLOCKS, LIGHT SHALL REMAINS ON</p> <p>NOMENCLATURE F. D1: ENTRY DOOR G. D2: EXIT DOOR</p> <p>IN NORMAL CONDITION, DOOR D1 AND D2 ARE IN UNLOCK CONDITION.</p> <p>FOR UNIT ON - MAINS ON - TUBELIGHT GETS ON BY ROTARY SWITCH</p> <p>DETAILS OF LOGIC SEQUENCE <u>FOR ONE SIDE ENTRY</u> FIRST CYCLE OF OPERATION – <ul style="list-style-type: none"> a) WHEN DOOR D1 IS OPENED DOOR D2 GETS LOCKED BLOWER IS IN OFF CONDITION b) DOOR D1 IS CLOSED, THEN DOOR D2 GETS LOCKED AND BLOWER MOTOR GETS ON BOTH DOORS ARE LOCK c) BLOWER MOTOR (AS PER TIMER SETTING 0-120 SEC) GETS OFF, THEN DOOR D2 GETS OPENED/UNLOCKED D1 LOCKED d) DOOR D2 IS CLOSED DOOR D1 AND D2 GETS OPENED/UNLOCKED BLOWER GETS OFF D1 LOCK – (ONE TIME ONE DOOR OPEN - D1 OPEN – D2 LOCK D2 OPEN –D1 LOCK <p style="text-align: center;">OR</p> <p><u>FOR BOTH SIDE ENTRY</u> SAME SEQUENCE OF OPERATION IS REPEATED FOR FURTHER CYCLE OF OPERATION</p> <p>GREEN INDICATION - OPEN RED INDICATION – LOCK</p> </p>

12.	ELECTRICALS	<ul style="list-style-type: none"> * ON/OFF SWITCHES FOR OPERATING B/MOTOR, TUBE LIGHT AND AUXILLARY SOCKET * AUTOMATIC DOOR INTERLOCKING SYSTEM ALONG WITH ELECTROMAGNETS, TIMER, MAGNETIC STRIP, EMERGENCY RELEASE SWITCH AND DOOR INDICATOR IS PROVIDED * LIGHT – 20 W, PHILLIPS MAKE FLUROSCENT TUBE – 01 NO. * 3 CORE CONNECTION CABLE – 3 METER LONG * REQUIRED SUPPLY – 415 V, 3 PHASE, 50 HZ.
13.	FEATURES	* FLOORING – SS PERFORATION
14.	DOCUMENTATION	DESIGN QUALIFICATION OPERATIONAL QUALIFICATION INSTALLATION QUALIFICATION PERFORMANCE QUALIFICATION
15.	TEST CERTIFICATES	MOC TEST CERTIFICATE MOTOR BLOWER TEST CERTIFICATE HEPA FILTER TEST CERTIFICATE PRE FILTER TEST CERTIFICATE

**TECHNICAL SPECIFICATIONS FOR GARMENT CABINET AT MAIN ENTRY
BEFORE AIR SHOWER AT GROUND FLOOR.**

1.	ITEM	GARMENT CABINET OF SIZE 4'X2'X4'
2.	MOC	SS 304, MATT FINISH
3.	CLASS	100
4.	QUANTITY	01 NO.
5.	SIZE	OVERALL DIM: 1370 (W) X 760 (D) X 2350 (H) MM WORKSPACE DIM : 1270 (W) X 650 (D) X 1220 (H) MM
6.	VELOCITY	90 \pm 20 FPM AT 6'' FROM FILTER FACE
7.	SUPPLY FILTER	MINIPLEAT HEPA AIR FILTER EFFICIENCY : 99.997% DOWN TO 0.3 MICRON GRADE : H - 14 MEDIA : MICRO GLASS FIBRE PAPER (IMPORTED) INITIAL P.D. : 15 MM OF W.G. FINAL P.D. : 40 MM OF W.G. SEPERATOR : HOT MELT GLOVE SEALING : EPOXY BASED PU ADHESIVE CASING : FACTORY EXTRUDED AL. SECTION, BOX TYPE SIZE : 1220 (W) X 610 (D) X 70 (H) MM – 01 NO.
8.	PRE FILTER	PRE FILTER FOR PRIMARY SUCTION GRADE : F7 GRADE AS PER BSEN 779 INITIAL P.D. : 6.5 MM OF W.G. FINAL P.D. : 13.0 MM OF W.G. SEPERATOR : ALUMINIUM SEALING : EPOXY BASED PU ADHESIVE CASING : ALUMINIUM ANODISED FLANGE TYPE
9.	BLOWER MOTOR ASSEMBLY	ELECTRIC MOTOR - 0.5 HP, 1 PHASE, 1400 RPM 230 V, 50 HZ – 01 NO. ALUMINIUM IMPELLER – 7 ½ '' X 4 ½'', STATISTICALLY ANDDYNAMICALLYBALANCEDALUMINIUM IMPELLERS – 01 SET (L+R) BLOWER CASING – FRP BLOWER CASING
10.	DOORS	HINGE TYPE DOOR WITH GLASS VIEW WINDOW, HANDLES, HINGES AND GASKET
11.	PRESSURE GAUGE	SENSOCON, USA MAKE MAGNEHELIC GAUGE RANGE : 0 – 50 MM OF W.G. SUITABLE TO CHECK THE PRESSURE DROP ACROSS THE HEPA FILTER - 01 NO.

- 5 -

12.	ELECTRICALS	<ul style="list-style-type: none"> * ROCKER SWITCHES FOR OPERATING B/MOTOR THAT THE UNIT REMAINS ON EVEN AFTER POWER FAILURE. * 3 CORE CONNECTION CABLE – 3 METER LONG * REQUIRED SUPPLY – 230 V, 1 PHASE, 50 HZ.
13.	FEATURES	<ul style="list-style-type: none"> * HANGER BAR * UV TUBE 15 W WITH HOUR METER - 01 NO. * TWO PERFORATED SHELFs ARE PROVIDED FOR SHOES AND CAPS * DOP TEST PORT * CASTOR WHEEL (FRONT SIDE LOCKABLE TYPE) AND LEVELLING BOLTS
14.	TESTING AND VALIDATION ON SITE	<p>HEPA FILTER LEAK TEST (DOP TEST) PARTICLE COUNT TEST FOR WORKING AREA VELOCITY TEST</p>
15.	DOCUMENTATION	<p>DESIGN QUALIFICATION OPERATIONAL QUALIFICATION INSTALLATION QUALIFICATION PERFORMANCE QUALIFICATION</p>
16.	TEST CERTIFICATES	<p>MOC TEST CERTIFICATE MOTOR BLOWER TEST CERTIFICATE MAGNEHELIC GAUGE CALIBRATION CERTIFICATE HEPA FILTER TEST CERTIFICATE PRE FILTER TEST CERTIFICATE</p>

TECHNICAL SPECIFICATIONS FOR GARMENT CABINET AT ENTRY BEFORE AIR SHOWER AT FIRST FLOOR AND SECOND FLOOR. ALSO AT SKID AND NUDE MICE LAB ON FIRST FLOOR AND SECOND FLOOR.


1.	ITEM	GARMENT CABINET OF SIZE 3'X2'X4'
2.	MOC	SS 304, MATT FINISH
3.	CLASS	100
4.	QUANTITY	01 NO.
5.	SIZE	WORKSPACE DIM : 965 (W) X 660 (D) X 1220 (H) MM OVERALL DIM: 1065 (W) X 760 (D) X 2350 (H) MM
6.	VELOCITY	90 ± 20 FPM AT 6" FROM FILTER FACE
7.	SUPPLY FILTER	MINIPLEAT HEPA AIR FILTER EFFICIENCY : 99.997% DOWN TO 0.3 MICRON GRADE : H - 14 MEDIA : MICRO GLASS FIBRE PAPER (IMPORTED) INITIAL P.D. : 15 MM OF W.G. FINAL P.D. : 40 MM OF W.G. SEPERATOR : HOT MELT GLOVE SEALING : EPOXY BASED PU ADHESIVE CASING : FACTORY EXTRUDED AL. SECTION, BOX TYPE SIZE : 915 (W) X 610 (D) X 70 (H) MM – 01 NO.
8.	PRE FILTER	PRE FILTER FOR PRIMARY SUCTION GRADE : F7 GRADE AS PER BSEN 779 INITIAL P.D. : 6.5 MM OF W.G. FINAL P.D. : 13.0 MM OF W.G. SEPERATOR : ALUMINIUM SEALING : EPOXY BASED PU ADHESIVE CASING : ALUMINIUM ANODISED FLANGE TYPE
9.	BLOWER MOTOR ASSEMBLY	ELECTRIC MOTOR - 0.5 HP, 1 PHASE, 1400 RPM 230 V, 50 HZ – 01 NO. ALUMINIUM IMPELLER – 7 ½" X 4 ½", STATISTICALLY AND DYNAMICALLY BALANCED ALUMINIUM IMPELLERS – 01 SET (L+R) BLOWER CASING – FRP BLOWER CASING
10.	DOORS	HINGE TYPE DOOR WITH GLASS VIEW WINDOW, HANDLES, HINGES AND GASKET
11.	PRESSURE GAUGE	SENSOCON, USA MAKE MAGNEHELIC GAUGE RANGE : 0 – 50 MM OF W.G. SUITABLE TO CHECK THE PRESSURE DROP ACROSS THE HEPA FILTER - 01 NO.


IISRE PUNE : AIR SHOWER AND GARMENT CABINET SPECIFICATIONS

Page 4 of 5



- 5 -

12.	ELECTRICALS	<ul style="list-style-type: none"> * ROCKER SWITCHES FOR OPERATING B/MOTOR THAT THE UNIT REMAINS ON EVEN AFTER POWER FAILURE. * 3 CORE CONNECTION CABLE – 3 METER LONG * REQUIRED SUPPLY – 230 V, 1 PHASE, 50 HZ.
13.	FEATURES	<ul style="list-style-type: none"> * HANGER BAR * UV TUBE 15 W WITH HOUR METER - 01 NO. * TWO PERFORATED SHELFs ARE PROVIDED FOR SHOES AND CAPS * DOP TEST PORT * CASTOR WHEELS (FRONT SIDE LOCKABLE TYPE) AND LEVELLING BOLTS
14.	TESTING AND VALIDATION ON SITE	<ul style="list-style-type: none"> HEPA FILTER LEAK TEST (DOP TEST) PARTICLE COUNT TEST FOR WORKING AREA VELOCITY TEST
15.	DOCUMENTATION	<ul style="list-style-type: none"> DESIGN QUALIFICATION OPERATIONAL QUALIFICATION INSTALLATION QUALIFICATION PERFORMANCE QUALIFICATION
16.	TEST CERTIFICATES	<ul style="list-style-type: none"> MOC TEST CERTIFICATE MOTOR BLOWER TEST CERTIFICATE MAGNEHELIC GAUGE CALIBRATION CERTIFICATE HEPA FILTER TEST CERTIFICATE PRE FILTER TEST CERTIFICATE

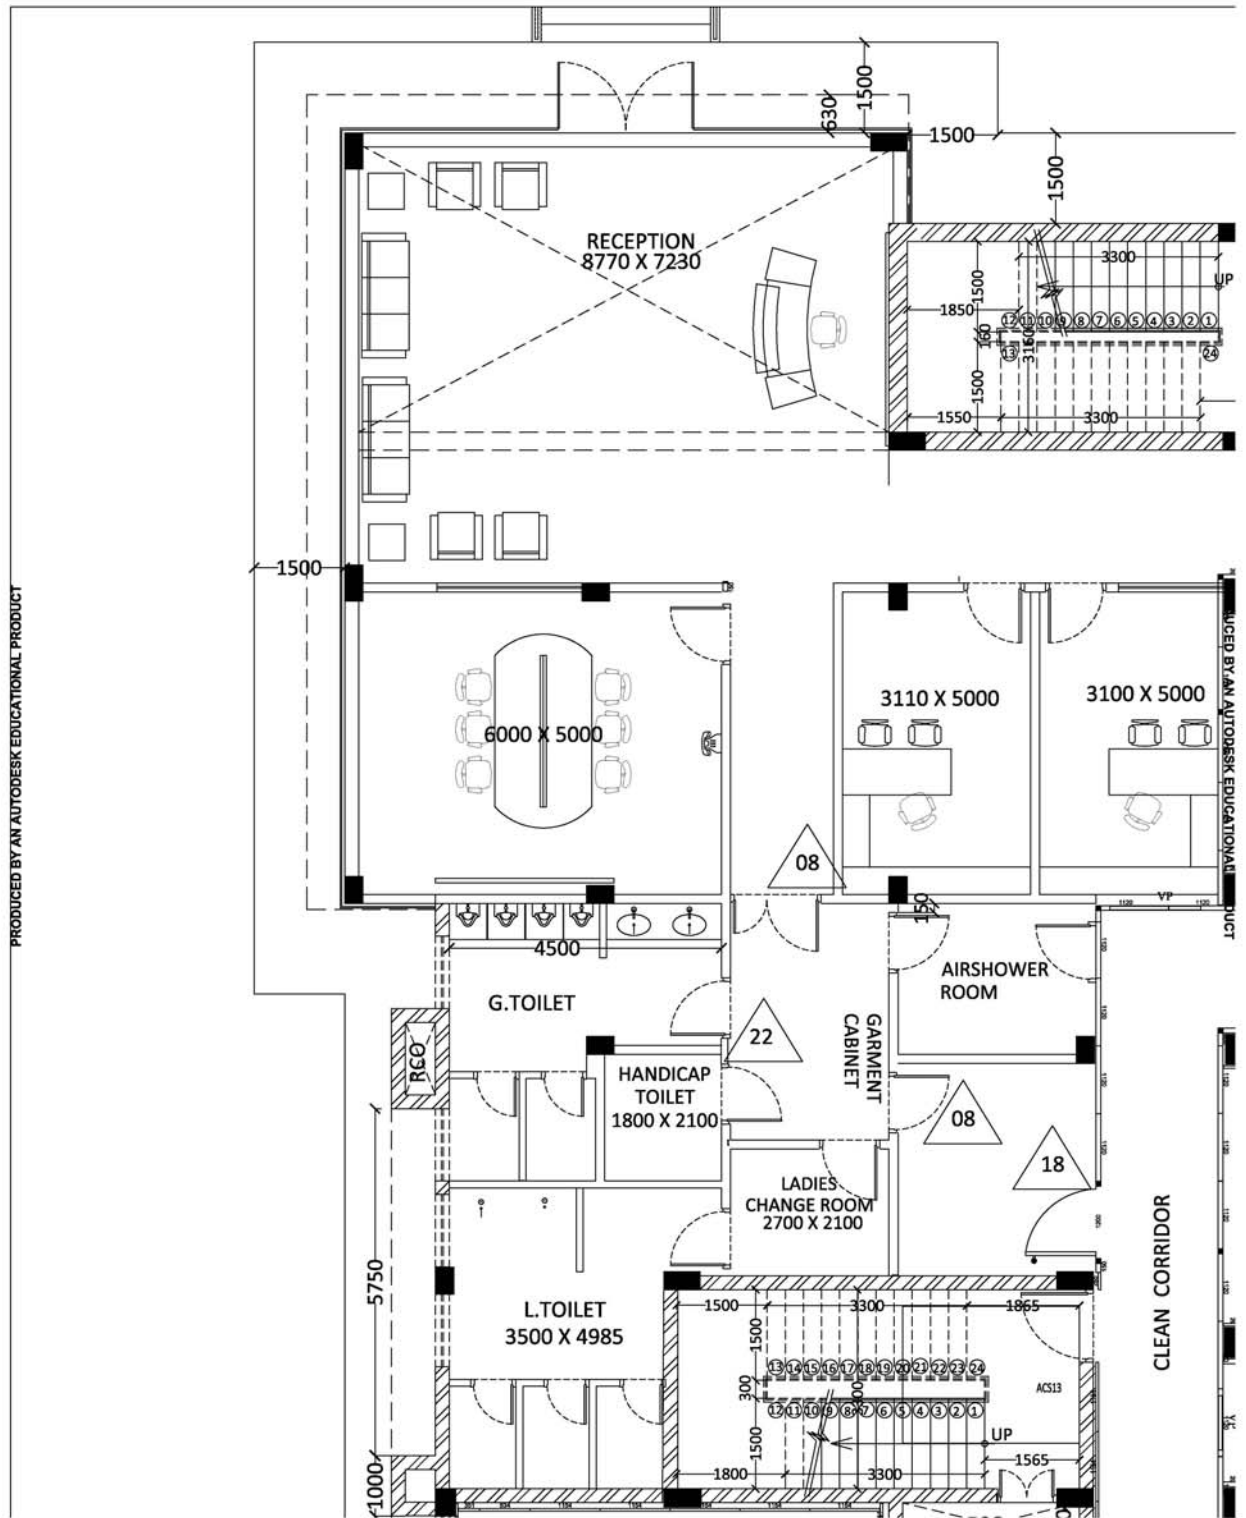



AIR SHOWER UNIT



SS 304 BOTTOM PLATE



PART DETAILS:-

- 1) AIR SUPPLY DUCTS
- 2) SUPPLY FILTER
- 3) B/W ASSEMBLY
- 4) PRE FILTER
- 5) INDICATION PLATE
- 6) DOOR CLOSER

TECHNICAL DETAILS:-

1. MOC : SS 304, MATT FINISH ON INNER SIDE
CROA POWDER COATED ON OUTER SIDE
COLOUR-RAL 9002 (OFFWHITE)
2. CLASS : 100
3. SUPPLY FILTER : MANUFACTURED HEPA FILTER - H14
99.997% DOWN TO 0.3 MICRON
CASING AL FACTORY EXTRUDED SECTION
AS PER IES-RP-CC-003
610X610X100 MM-01 NO
610X915X100 MM-02 NO
4. PRE FILTER : F7 GRADE AS PER BSEN 779
ALUMINIUM FLANGE TYPE
FLANGE-695X395 BOX-630X330X50 MM-01 NO
FLANGE-1195X395 BOX-1130X330X50 MM-01 NO
5. B/W ASSLY : 1 HP, 3 PHASE, 2880 RPM, DOUBLE SHAFT
415 V AC, 50 HZ, HINDUSTAN MAKE-02 NOS
C/IMPELLER 75X45
FRP BLOWER CASING WITH REXINE CONNECTOR
AND ANTIVIBRATION MOUNTING
6. VELOCITY : AT NOZZLE 30 M/SEC
TOTAL 29 NOZZLES-23 NOS AT RIGHT+LEFT SIDE,
6 NOS. ON TOP SIDE
7. DOOR : SS 304 DOOR 3 NOS WITH HALF GLASS VIEW
WINDOW, DOOR CLOSER, HANDLES, HINGES,
INTERLOCKING SYSTEM FOR THREE SIDE ENTRY
AND EXIT DOOR
8. CONTROL LOGIC : PROGRAMMABLE LOGIC CONTROLLER (PLC)
ACTIVATING THE EMERGENCY SWITCH SHALL CAUSE
THE CYCLE TO IMMEDIATELY END AND RELEASE
ALL INTERLOCKS, LIGHT SHALL REMAINS ON
9. FEATURES : HANDLES TUBELIGHT 14W (2)-02 NOS.
FLOORING-PERFORATED SS SHEET
10. QUANTITY : 01 NO

INTERNAL DIMENSION :- 800(W) X 1680(D) X 2050(H) MM
EXTERNAL DIMENSION :- 1500(W) X 2160(D) X 2150(H) MM


CLIENT:- I I S E R : PUNE


REF:-

DRAWING NO.:- AISA025

SURFACE FINISH SYMBOLS


SCALE:- 1:1	REVISION	DATE	BY	CHECKED	APPROVED
REV:- 00	DATE:- 19.05.16				
ALL DIMENSIONS ARE IN MM					

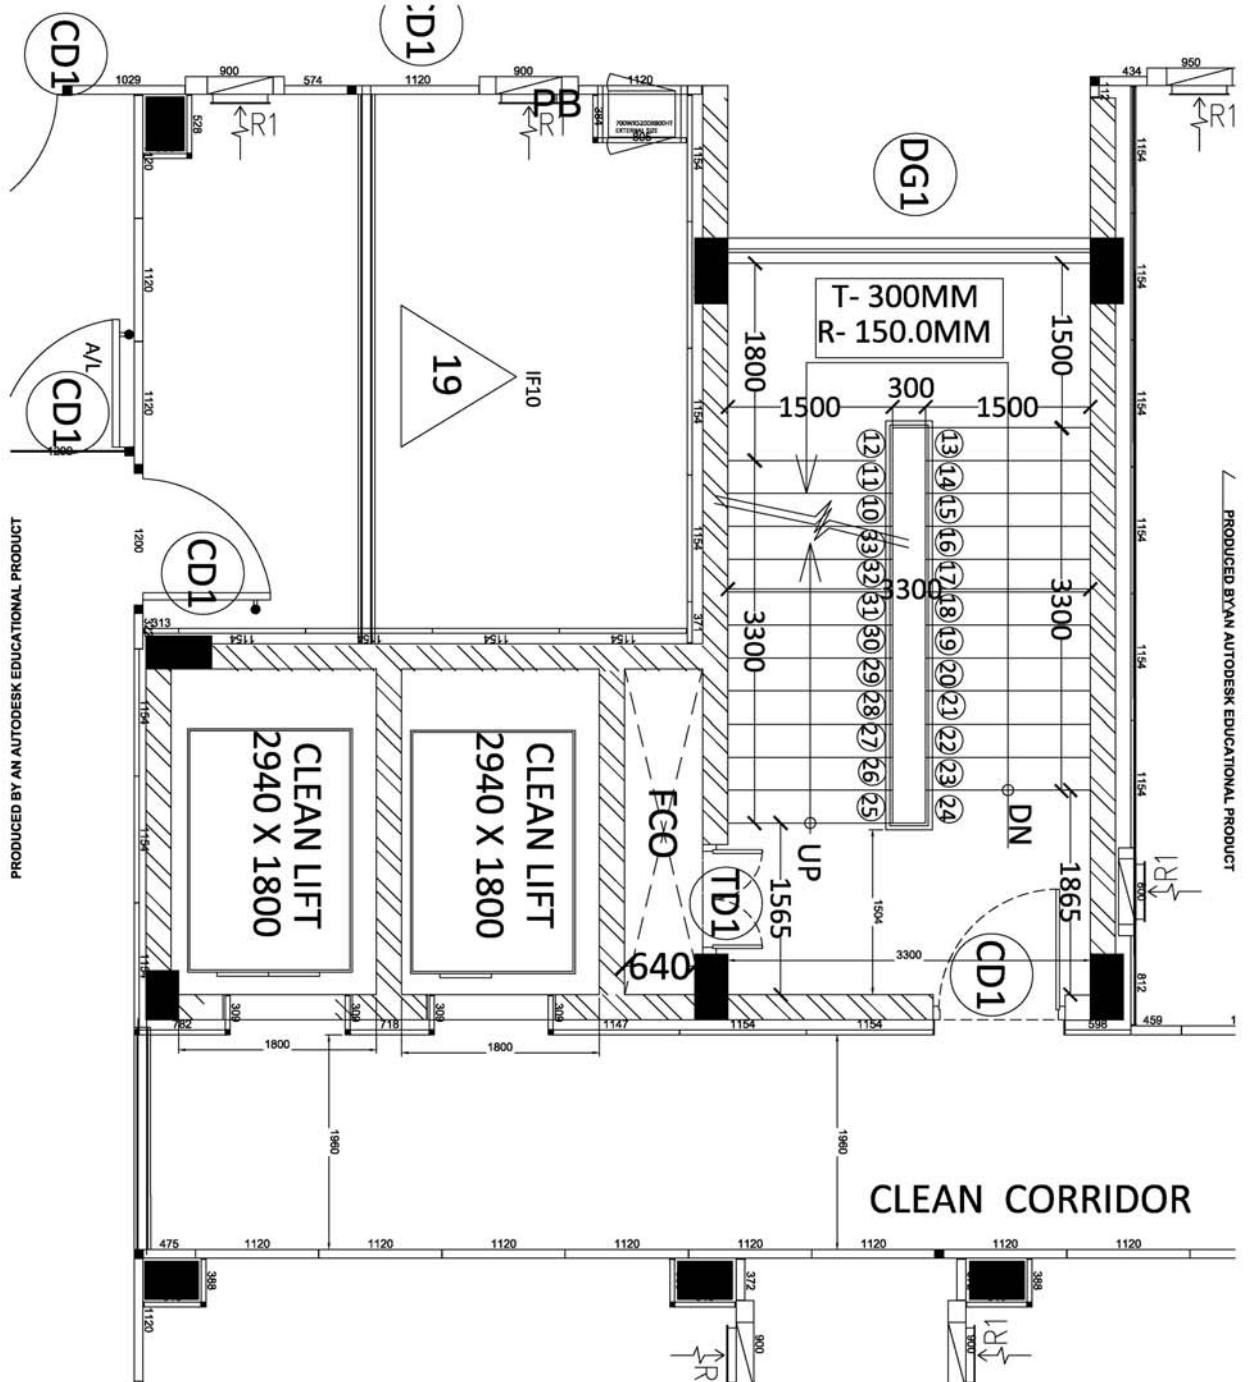

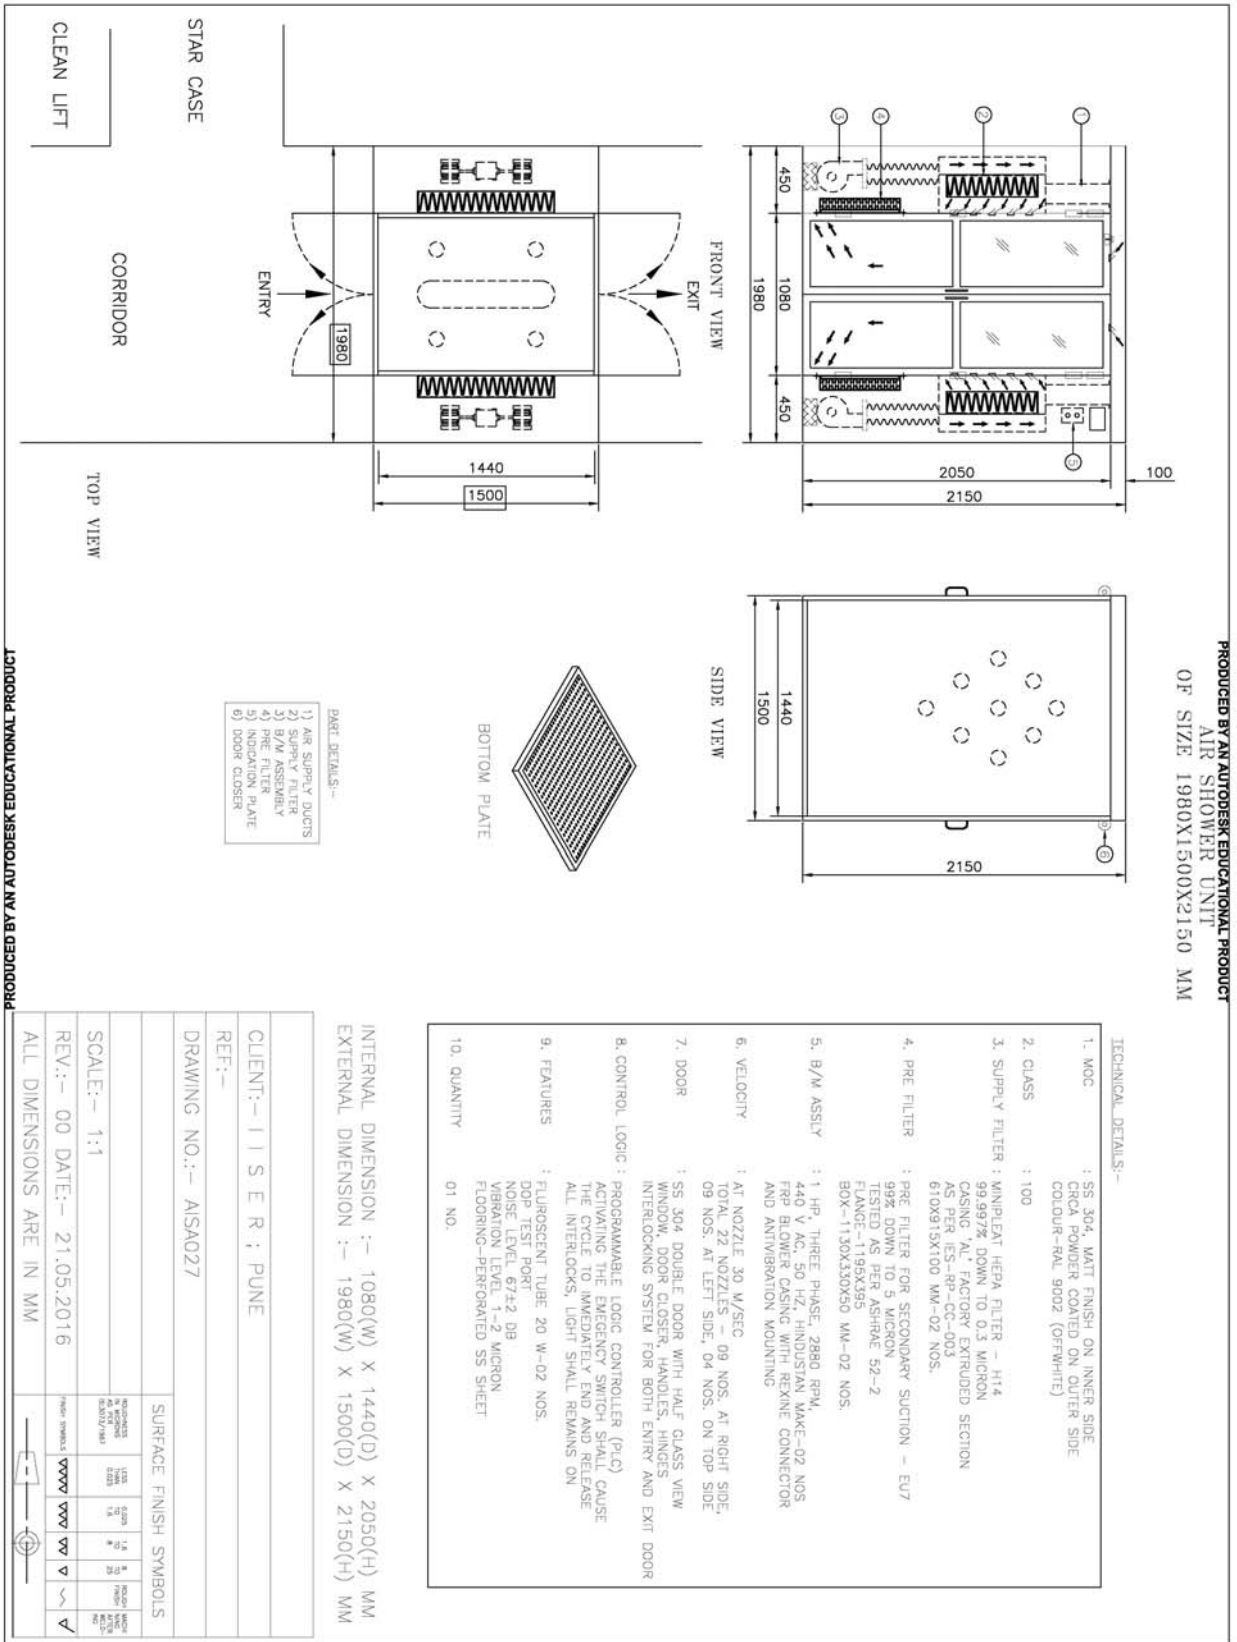

SLIDING TYPE DOOR

GARMENT CABINET - CLASS 100
OF SIZE 4'X2'X4'



TECHNICAL SPECIFICATIONS :	
MOCC	: SS 304, MATT FINISH
GLASS	: 100
VELOCITY	: 90 - 110 FPM AT 6" FROM FILTER FACE
SUPPLY FILTER	: MINIPLEX HEPA FILTER-H14 99.997% DOWN TO 0.3 MICRON CASING ALUMINUM FACTORY EXTRUDED SECTION ALUMINUM BOX TYPE 15" SQUARE FILTER ES RP-003 1220X610X10 MM-01 NO.
PHE FILTER	: F7 GRADE AS PER BS EN 779 ALUMINUM ANODISED FLANGE TYPE BOX 1050X1850X9 MM-01 NO.
B/N ASSEMBLY	: 0.5 HP ELEC. MOTOR CAPTION MAKE 1440 RPM, 230 V, SINGLE PHASE, 50 HZ W/ BLOWER WITH ALUMINUM IMPELLER 725X92 DOUBLE SHIRT
DOOR	: SLIDING TYPE DOOR WITH GLASS VIEW WINDOW IN SS FRAME
ELEC. SUPPLY AND ACCESSORIES	: ON/OFF SWITCH FOR B/MOTOR AND TUBE LIGHT 230 V, SINGLE PHASE, 50 HZ UV LIGHT 15 W WITH HOUR METER
PRESSURE GAUGE	: MAGNETIC GAUGE RANGE 0-50 MM W.G. DRYER MAKE-01 NO.
FEATURES	: INACER BAR FOUR PERFORATED SHELVES ARE PROVIDED FOR SHOES AND GAYS DOOR IS OPENED BY DOOR TEST PORT CASTOR WHEELS (FRONT SIDE LOCKABLE TYPE) AND LEVELLING BOLTS
QUANTITY	: 01 NO.


WORKSPACE DIM.: 1270(W) X 660(D) X 1220(H) MM
OVERALL DIM.: 1370(W) X 760(D) X 2350(H) MM

CLIENT:- I I S E R : PUNE	
DRAWING NO.:- 6221	
SURFACE FINISH SYMBOLS	
 MACHINED SURFACE BY TURNING BY MILLING BY GRINDING BY PLANING BY BROTHING BY SHARPENING BY POLISHING BY OTHER MEANS	 CAST SURFACE BY SAND CASTING BY DIE CASTING BY OTHER MEANS
 HOT-ROLLED SURFACE BY HOT-ROLLING BY OTHER MEANS	 COLD-ROLLED SURFACE BY COLD-ROLLING BY OTHER MEANS
 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS	 AS-FORGED SURFACE BY FORGING BY OTHER MEANS
 AS-CAST SURFACE BY SAND CASTING BY DIE CASTING BY OTHER MEANS	 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS
 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS	 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS
 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS	 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS
 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS	 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS
 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS	 AS-ROLLED SURFACE BY HOT-ROLLING BY COLD-ROLLING BY OTHER MEANS

PRODUCED BY AN AUTODESK EDUCATIONAL PRODUCT

PRODUCED BY AN AUTODESK EDUCATIONAL PRODUCT

GARMENT CABINET – CLASS 100 OF SIZE 3'X2'X4'



QUANTITY:- 01 NO.

TECHNICAL DETAILS:-	
S.R. NO.	PART DETAILS
1)	MAIN CUBICAL-SS 304, MATT FINISH
2)	PRE FILTER – F6 GRADE AS PER BSEN 779
3)	ALUMINIUM ANODISED FLANGE TYPE ELECTRIC SWITCH
4)	BLOWER MOTOR ASSEMBLY 0.5 HP ELEC. MOTOR CROMPTON MAKE 1440 RPM, 230 V, SINGLE PHASE, 50 HZ FRP BLOWER WITH ALUMINIUM IMPELLER 78X48 DOUBLE SHAFT
5)	SUPPLY FILTER-MINIPLEAT HEPA FILTER 99.997% DOWN TO 0.3 MICRON 'AL' FACTORY EXTRUDED AS PER IES RP 003 SIZE: 915X610X70 MM-01 NO.
6)	U/V TUBE (1SW)
7)	HANGER BAR
8)	HANDLE
9)	DOOR-HINGE TYPE GLASS DOOR
10)	PRESSURE GAUGE-DWYER MAKE MINIHILIC GAUGE 0-50 MM
11)	HOOR METER
12)	CASTOR WHEELS
13)	LEVELLING BOLTS

FEATURES: TWO PERFORATED SHELF IS PROVIDED FOR SHOES AND CAPS

ISOMETRIC VIEW

FRONT VIEW

SIDE VIEW

TOP VIEW

PRODUCED BY AN AUTODESK EDUCATIONAL PRODUCT

PRODUCED BY AN AUTODESK EDUCATIONAL PRODUCT

INTERNAL DIM. :- 965 (W)X660 (D)X1220 (H) MM	
EXTERNAL DIM.:- 1065 (W)X760 (D)X2450 (H) MM	
CLIENT:- I I S E R : PUNE	
DRAWING NO.:- 6114	
SCALE:- 1:1	
REV:- 00 DATE:- 05.09.2012	
ALL DIMENSIONS ARE IN MM	
SURFACE FINISH STANDARDS	
AL. DIMENSIONS ARE IN MM	

The Indian Institute of Science Education and Research (IISER-Pune)

BILL OF QUANTITY

Sr.No.	Item Description	Quantity	Unit	Rate in figure and words	Amount
1	Air shower at Main Entry of Clean Corridor of GF-Animal House facility as per attached details for size OVERALL DIM : 2400 (W) X 3100 (D) X 2150 (H) MM WORK-SPACE DIM : 1500 (W) X 3040 (D) X 2050 (H) MM	1	EACH		
2	Air shower at Entry of First Floor of Clean Corridor of Animal house facility as per details as attached. OVERALL DIM : 1980 (W) X 1500 (D) X 2150 (H) MM WORKSPACE DIM : 1080 (W) X 1440 (D) X 2050 (H) MM	1	EACH		
3	Air shower Entry of Second Floor of Clean Corridor of Animal house facility as per details as attached. OVERALL DIM : 1980 (W) X 1500 (D) X 2150 (H) MM WORKSPACE DIM : 1080 (W) X 1440 (D) X 2050 (H) MM	1	EACH		

Sr.No.	Item Description	Quantity	Unit	Rate in figure and words	Amount
4	Air shower at Entry of Skid Mice Lab at First Floor of Clean area-Animal House facility as per details as attached. OVERALL DIM : 1500 (W) X 2000 (D) X 2150 (H) MM WORKSPACE DIM : 800 (W) X 1940 (D) X 2050 (H) MM with 2 Exit doors.	1	EACH		
5	Air shower at Entry of Skid Mice Lab at Second Floor of Clean area-Animal House facility as per details as attached. OVERALL DIM : 1500 (W) X 2000 (D) X 2150 (H) MM WORKSPACE DIM : 800 (W) X 1940 (D) X 2050 (H) MM with 2 Exit doors.	1	EACH		
6	Garment box at Main Entry of Clean Corridor of GF-Animal House facility as per attached details. OVERALL DIM : 1370 (W) X 760 (D) X 2350 (H) MM WORKSPACE DIM : 1270 (W) X 650 (D) X 1220 (H) MM	1	EACH		
7	Garment box at Entry of First Floor of Clean Corridor of Animal house facility as per details as attached. WORKSPACE DIM : 965 (W) X 660 (D) X 1220 (H) MM OVERALL DIM : 1065 (W) X 760 (D) X 2350 (H) MM	1	EACH		

--	--	--	--	--	--	--

Sr.No.	Item Description	Quantity	Unit	Rate in figure and words	Amount
8	Garment box at Entry of Second Floor of Clean Corridor of Animal house facility as per details as attached. WORKSPACE DIM : 965 (W) X 660 (D) X 1220 (H) MM OVERALL DIM : 1065 (W) X 760 (D) X 2350 (H) MM	1	EACH		
9	Garment box at Entry of Skid Mice Lab at First Floor of Clean area-Animal House facility as per details as attached. WORKSPACE DIM : 965 (W) X 660 (D) X 1220 (H) MM OVERALL DIM : 1065 (W) X 760 (D) X 2350 (H) MM	1	EACH		
10	Garment box at Entry of Skid Mice Lab at Second Floor of Clean area-Animal House facility as per details as attached. WORKSPACE DIM : 965 (W) X 660 (D) X 1220 (H) MM OVERALL DIM : 1065 (W) X 760 (D) X 2350 (H) MM	1	EACH		
	TOTAL				

Note:

- (a) Indian agents name & address _____
- (b) Installation, commissioning & training charges, if any _____
- (c) Cost of Spares _____
- (d) The Indian agent's commission shall paid in Indian Rupees only based on the Exchange Rate prevailing on the date of negotiation of documents.
- (e) The cost of optional items shall be indicated separately.

PRICE SCHEDULE FOR GOODS BEING OFFERED FROM INDIA

Name of the Bidder _____

Tender No. _____

1	2	3	4	5	6	7	8	9	10	11
Sl. No.	Item Description	Country of Origin	Unit	Qty	Ex-Works. Ex-Warehouse, Ex-show room off the shelf price (inclusive of all taxes already paid)	Total price Ex-Works. Ex-Warehouse, Ex-show room off the shelf price (inclusive of all taxes already paid) 5x6	VAT & other taxes like excise duty payable, if contract is awarded	Packing & forwarding up to station of dispatch, if any	Charges of inland transportation, insurance up to Lab./Instt.	Installation, Commissioning & training charges, If any.



1	2	3	4	5	6	7	8	9	10	11

Total Bid price in foreign Currency _____ in words.

Signature of Bidder :

Name :

Note:

The cost of optional items shall be indicated separately.

(a) Cost of spares _____

FORMAT/QUESTIONNAIR FOR COMPLIANCE OF TERMS AND CONDITIONS

Tender No.: _____

Due

Date _____

NOTE:

3. Quotation will not be considered without submission of this format.
4. If a particular question is not at all applicable please write NA in compliance part in Col. No. 4 below.
5. Kindly see the relevant terms & conditions of the tender document in each question before replying to the questions mentioned in Col. 2 below).

SNo	Terms & condition of Tender document	Whether acceptable (say 'Yes' or 'No' (preferably use different colour ink for 'No'))	Deviation from tender terms, if any, with reasons for noncompliance or alternative condition quoted for
1	2	3	4
1	a.) Whether quotation is direct from Principal supplier/manufacturer or their own office in India (Please specify)		
	b) Whether quotation is being submitted by Indian Agent/authorized distributor/ dealer		
	c) Whether the agent is registered with DGS&D/NSIC		
2	a) Whether the Techno-commercial and price bids (for two bid tender system only) have been kept in separate envelopes duly marked with "Techno-commercial Bid" and "Price Bids" respectively.		
	b) Whether the tender No., Due date & Opening dates have been written outside all the envelopes.		
3	Whether techno-commercial Bid contains EMD, technical literature/leaflets, detailed specifications & commercial terms & conditions etc. as applicable.		
4	a) Whether the required EMD is being submitted with the quotation		

SNo	Terms & condition of Tender document	Whether acceptable (say 'Yes' or 'No' (preferably use different colour ink for 'No'))	Deviation from tender terms, if any, with reasons for noncompliance or alternative condition quoted for
	b) Please specify the form of EMD whether in the form of DD/bank guarantee or TDR/FDR (Please mention No., date & amount of EMD documents.) or Bid Security		
	c) Pre-receipted bill for refund of EMD is enclosed (for bank drafts only)		
5	a. If the prices are on Ex-Works basis or FOB (names port of shipment) or FCA (named place of delivery abroad)		
	b. Whether specific amounts or percentage of expenses like packing, forwarding, handling, freight, insurance, documentation etc. have been mentioned in quotation separately in clear terms.		
6	a) Whether prevailing rates of sales tax, excise duty & other govt. levies (for indigenous supplies) have been given in quotation		
7	Have you mentioned the validity period of the quotation as per our requirements		
8	a) Whether the Price reasonability Certificate is submitted with quotation		
	b) Whether copies of last two supply orders of the same item from other customers have been attached with the quotation		
9	Whether rates/amount of AMC after the warranty period is over has been mentioned		
10	Have you gone through the specification Clause & complied with the same		

SNo	Terms & condition of Tender document	Whether acceptable (say 'Yes' or 'No' (preferably use different colour ink for 'No'))	Deviation from tender terms, if any, with reasons for noncompliance or alternative condition quoted for
11	Whether the Make/Brand, Model number and name of manufacturer has been mentioned in the quotation and Printed technical literature/ leaflets of quoted items have been submitted		
12	Whether compliance statement of specifications has been attached with the quotation.		
13	a) Whether the delivery period for supply of the items has been mentioned		
	b) Whether mode of delivery & tentative size & weight of the consignment has also been indicated		
14	Do you agree to the submission of Performance Bank Guarantee and have you mentioned in your quotation about this.		
15	a) Do you agree with the payment terms for indigenous supplies?		No deviation permitted
	b) Do you agree with the payment terms for imports supplies?		
16	Do you agree about the date of commencement of warranty period & its extension is necessary.		
17	a) Who will install/commission and demonstrate the equipment at IISER Pune, FREE OF COST.		
	b) Will you be able to do it within a month		
18	Have you mentioned the guarantee/warranty period in your quotation and do you agree with guarantee clause?		
19	Spare parts		
20	After Sales service		

SNo	Terms & condition of Tender document	Whether acceptable (say 'Yes' or 'No' (preferably use different colour ink for 'No'))	Deviation from tender terms, if any, with reasons for noncompliance or alternative condition quoted for
21	a) Do you agree that on receipt of material in damaged condition or short supply you will replace the same on CIF basis, free of cost pending the settlement of the		
	b) Do you agree with the clause of physical inspection?		
22	Whether list of specific user's for the same item & model as quoted along-with performance certificates from the users is submitted with offer		
23	Whether you agree to the penalty clause for late delivery & installation?		
24	Whether training to our scientist/technical person will be given free of cost . If yes, have you specified in quotation whether it will be in our lab? Or at supplier's site in India or abroad.		
25	a) Whether all the pages have been page numbered?		
	b) Whether quotation has been signed and designation & name of signatory mentioned.		

FORMAT OF COMPLIANCE STATEMENT OF SPECIFICATIONS

S. N.	Name of specifications/ part / Accessories of tender enquiry	Specifications of quoted Model/ Item	Compliance Whether “YES” Or “NO”	Deviation, if any, to be indicated in unambiguous terms	Whether the compliance / deviation is clearly mentioned in technical leaflet/ literature
1	2	3	4	5	6

BID SECURITY FORM

Whereas (Hereinafter called “the tenderer”) has submitted their offer dated for the supply of (Hereinafter called “the tender”) against the purchaser’s tender enquiry No. _____

KNOW ALL MEN by these presents that WE (Name of bank) of (Name of country), having our registered office at (Address of bank) (Hereinafter called the “Bank”), are bound unto ... (Name of purchaser) (Hereinafter called “the purchaser”) in the sum of for which payment will and truly to be made to the said Purchaser, the Bank binds itself, its successors, and assigns by these presents. Sealed with the Common Seal of the said Bank this day of 20.....

THE CONDITIONS OF THESE OBLIGATIONS ARE:

1. If the tenderer withdraws or amends, impairs or derogates from the tender in any respect within the period of validity of this tender.
2. If the tenderer having been notified of the acceptance of his tender by the Purchaser during the period of its validity.
3. If the tenderer fails to furnish the Performance Security for the due Performance of the contract.
4. Fails or refuses to accept/execute the contract.

WE undertake to pay the Purchaser up to the above amount upon receipt of its first written demand, without the Purchaser having to substantiate its demand, provided that in its demand the Purchase will note that the amount claimed by it is due to it, owing to the occurrence of one or both of the two conditions, specifying the occurred condition or conditions.

The guarantee shall remain in force up to and including forty five (45) days after the period of the bid validity, and any demand in respect thereof should reach the Bank not later than the above date.

.....
(Signature of the authorized officer of the Bank)

Name and Designation of the Officer
Seal, Name & Address of the Bank and address
of the branch

MANUFACTURER’S AUTHORIZATION FORM

[The Bidder shall require the Manufacturer to fill in this Form in accordance with the instructions indicated. This letter of authorization should be on the letterhead of the Manufacturer and should be signed by a person with the proper authority to sign documents that re binding on the Manufacturer]

Date: *[Insert date (as Day, month and year) of Bid submission]*

Tender No.: *[Insert number from Invitation for Bids]*

To: *[Insert complete name and address of Purchaser]*

WHEREAS

We *[insert completer name of Manufacturer]*, who are official manufacturers of *[Insert type of goods manufactured]* having factories at *[insert full address of Manufacturer’s factories]*, do hereby authorize *[insert complete name of Bidder]* to submit a bid the purpose of which is to provide the following goods, manufactured by us *[insert name and or brief description of the goods]*, and to subsequently negotiate and sign the contract.

We hereby extend our full guarantee and warranty in accordance with the Terms and Conditions of Contract with respect to the Goods offered by the above firm.

Signed: *[insert signature(s) of authorized representative(s) of the Manufacturer]*

Name: *[insert complete name(s) of authorized representative(s) of the Manufacturer]*

Title: *[insert title]*

Duly authorized to sign this Authorization on behalf of: *[insert complete name of Bidder]*

Dated on _____ day of _____ *[insert date of signing]*

PREVIOUS SUPPLY ORDERS FORMAT

Name of the Firm _____

Order placed by {Full address of Purchaser]	Order No. and Date	Description and quantity of ordered equipment	Value of order	Date of completion of delivery as per contract	Date of actual completion of delivery	Remarks indicating reasons for late delivery, if any and justification for price difference of their supply order & those quoted to us.	Has the equipment been installed satisfactorily ? <i>(Attach a certificate from the Purchaser/ Consigner]</i>	Contact Person along with Telephone no., Fax no. and e-mail address.

Signature and Seal of the Manufacturer/ bidder

Place:

Date:

BIDDER INFORMATION FORM

Company Name : _____
 Registration Number : _____
 Registered Address : _____

Name of Partners /Director : _____

City : _____
 Postal Code : _____

Company's Establishment Year : _____

Company's Nature of Business : _____

Company's Legal Status (tick on appropriate option)

- 1) Limited Company
- 2) Undertaking
- 3) Joint Venture
- 4) Partnership
- 5) Others

Company Category

- 1) Micro Unit as per MSME
- 2) Small Unit as per MSME
- 3) Medium Unit as per MSME
- 4) Ancillary Unit
- 5) SSI
- 6) Others

CONTACT DETAILS

Contact Name : _____
 Date of Birth : _____
 Email Id : _____
 Designation : _____
 Phone No : (_____) _____

Mobile No : _____

BANK DETAILS

Name of Beneficiary : _____

A/c. No. CC/CD/SB/OD: _____

Name of Bank : _____

IFSC NO. (Bank) : _____

Branch Address and Branch Code: _____

Other Details

Vendor's PAN No. _____

Vendor's CST No/LST No/WCT No/TIN No: _____

Checklist for BIDDERS

BIDDERS to indicate whether the following are enclosed / mentioned by striking out the non-relevant option and write concern page no.

S. No	Particulars	Documents Attached	Page No
1	Two separate bids duly filled in and signed in sealed envelopes (i) Technical (ii) Commercial	(Yes / No)	
2	The Demand Draft/BG for Rs 62,000/- towards Earnest Money Deposit	(Yes / No)	
3	Format/Questionnaire For Compliance Of Terms And Conditions Annexure – A	(Yes / No)	
4	Format of compliance statement of specifications - Annexure – B	(Yes / No)	
5	Bid Security Form - Annexure – C (as applicable)	(Yes / No)	
6	Manufacturer's Authorization Form - Annexure – D	(Yes / No)	
7	Previous Supply Orders - Annexure – E	(Yes / No)	
8	Bidder Information form - Annexure – F	(Yes / No)	
9	A copy of the Un-priced Commercial bid	(Yes / No)	
10	List of deliverables as per Chapter- 4	(Yes / No)	
11	Solvency certificate for Rs 12.40 lakhs (not older than twelve months) issued by scheduled/nationalized bank with which BIDDER holds the current account	(Yes / No)	
12	Undertaking that the successful BIDDER agrees to give a 10 % security deposit and Performance Bank Guarantee	(Yes / No)	
13	Self Attested copy of Sales Tax Registration certificate (CST/VAT etc) (as applicable)	(Yes / No)	
14	Delivery Period, Warranty and Payment terms are clearly mentioned	(Yes / No)	
15	Acceptance of IISER, PUNE Cargo Agent	(Yes / No)	
16	Bank charges agreed for outside India	(Yes / No)	
17	LD clause agreeable.	(Yes / No)	
18	Supply of spares for 7 years	(Yes / No)	
19	Acceptance of warranty period and Free replacements during warranty period	(Yes / No)	
20	Amalgamation/Acquisition: Successor agreeable to fulfill the contractual obligations	(Yes / No)	
21	Tender Terms & Conditions Acceptance (last page) signed with official seal is attached	(Yes / No)	

IMPORTANT NOTICE

TENDERERS RESPONDING TO THIS ENQUIRY SHALL BE DEEMED TO BE AGREEABLE TO THE TERMS AND CONDITIONS HEREIN CONTAINED. THESE TERMS AND CONDITIONS SHALL BE BINDING ON THE SUCCESSFUL TENDERER. CONDITIONAL TENDERS ARE LIABLE TO BE REJECTED. IISER PUNE WILL PROCESS THE TENDER AS PER IISER PUNE STANDARD PROCEDURES. THE DIRECTOR OF THE INSTITUTE RESERVES THE RIGHT TO REJECT ANY OR ALL OR PART OF TENDER WITHOUT ASSIGNING ANY REASON AND SHALL ALSO NOT BE BOUND TO ACCEPT THE LOWEST TENDER. IISER PUNE WOULD NOT BE UNDER ANY OBLIGATION TO GIVE ANY CLARIFICATIONS TO THE AGENCIES WHOSE BIDS ARE REJECTED.

I agree to all terms and conditions mentioned in the tender document of the Institute

Signature of the Tenderer